

---

---

**Dentistry — Dental furnace —**

**Part 3:**

**Test method for the evaluation of  
high temperature sintering furnace  
measurement with a separate  
thermocouple**

*Médecine bucco-dentaire — Fours dentaires —*

*Partie 3: Méthode d'essai pour l'évaluation du mesurage des hautes  
températures de frittage au moyen d'un thermocouple externe*



STANDARDSISO.COM : Click to view the full PDF of ISO 13078-3:2023



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

|                                               | Page     |
|-----------------------------------------------|----------|
| Foreword.....                                 | iv       |
| Introduction.....                             | v        |
| <b>1 Scope.....</b>                           | <b>1</b> |
| <b>2 Normative references.....</b>            | <b>1</b> |
| <b>3 Terms and definitions.....</b>           | <b>1</b> |
| <b>4 Measurement and test method.....</b>     | <b>2</b> |
| 4.1 General.....                              | 2        |
| 4.2 Test devices and test equipment.....      | 2        |
| 4.2.1 Thermocouple fixture.....               | 2        |
| 4.2.2 Thermocouple.....                       | 3        |
| 4.2.3 Compensating cable.....                 | 3        |
| 4.2.4 Temperature indicating device.....      | 4        |
| 4.2.5 High temperature sintering furnace..... | 4        |
| 4.3 Implementation.....                       | 4        |
| 4.3.1 Layout of the thermocouple.....         | 4        |
| 4.3.2 Heating phase.....                      | 4        |
| 4.3.3 Test temperature 1.....                 | 4        |
| 4.3.4 Holding time 1.....                     | 4        |
| 4.3.5 First measurement.....                  | 4        |
| 4.3.6 Test temperature 2.....                 | 4        |
| 4.3.7 Holding time 2.....                     | 4        |
| 4.3.8 Second measurement.....                 | 4        |
| 4.3.9 Interpretation.....                     | 5        |
| 4.3.10 Adjustment.....                        | 5        |
| <b>5 Test report.....</b>                     | <b>5</b> |
| <b>Bibliography.....</b>                      | <b>6</b> |

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at [www.iso.org/patents](http://www.iso.org/patents). ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 2, *Prosthetic materials*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 55, *Dentistry*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

A list of all parts in the ISO 13078 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

## Introduction

In dentistry, sintering furnaces are used for sintering restorations made from oxide ceramics and from sintered metal. Significantly higher temperatures than those for firing dental ceramic masses containing silicates are necessary, for example, zirconium oxide ( $\text{ZrO}_2$ ) is typically sintered at a temperature of up to 1 700 °C.

The sintering temperature is of vital importance for the properties of the sintered material. Incorrect sintering temperatures can result in low strength, discrepant colouration or low ageing resistance. Furthermore, a poor accuracy of fit owing to excessively low or uneven shrinkage can occur. Too high a sintering temperature generally results in a larger grain size and can lead to a softening and consequently a deformation of the restoration. Too low a sintering temperature results in an inadequate sintering quality and possibly residual porosity.

STANDARDSISO.COM : Click to view the full PDF of ISO 13078-3:2023

STANDARDSISO.COM : Click to view the full PDF of ISO 13078-3:2023

# Dentistry — Dental furnace —

## Part 3:

# Test method for the evaluation of high temperature sintering furnace measurement with a separate thermocouple

## 1 Scope

This document specifies a test method for the calibration of resistance-heated high temperature sintering furnaces that are suitable for the sintering of dental restorations in the temperature range up to 1 700 °C.

**NOTE** A test method for the calibration of dental furnaces that are suitable for the heat treatment of silica-based dental ceramic restorations in the temperature range between 600 °C and 1 050 °C is specified in ISO 13078:2013. ISO 13078:2013 does not include the calibration of sintering furnace used for sintering of oxide ceramics or sintered metal, in whose firing chamber restorations are sintered at temperatures of 1 000 °C to 1 700 °C.

## 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942, *Dentistry — Vocabulary*

ISO 6872, *Dentistry — Ceramic materials*

IEC 60584-1:2013, *Thermocouples — Part 1: EMF specifications and tolerances*

IEC 60584-3, *Thermocouples — Part 3: Extension and compensating cables — Tolerances and identification system*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942, ISO 6872 and IEC 60584-1:2013 and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

### 3.1

#### heating rate

rate of temperature increase

Note 1 to entry: The heating rate shall be expressed in degrees Celsius per minute (°C/min).

### 3.2

#### **holding time**

time span in which the desired temperature of the *sintering* (3.5) furnace is retained up to the time specified by the manufacturer, beginning from the time point at which the display on the sintering furnace indicates that the sintering furnace has reached the desired temperature

### 3.3

#### **high temperature sintering furnace**

*sintering* (3.5) furnace, in whose firing chamber restorations are sintered at temperatures of 1 000 °C to 1 700 °C

### 3.4

#### **oxide ceramic**

ceramic produced from a crystalline feedstock powder at high temperatures via a *sintering* (3.5) process

Note 1 to entry: All ceramics which do not contain SiO<sub>2</sub> and which are exclusively oxidic are referred to as oxide ceramics.

Note 2 to entry: In contrast to this, ceramics containing SiO<sub>2</sub> are referred to as silicate ceramics. If ceramics contain not only oxygen as an electronegative component but also, for example, carbon or nitrogen, they shall be referred to as non-oxide ceramics. Only the oxide ceramics zirconium oxide and aluminium oxide as well as composites of these are common in dental technology at present.

### 3.5

#### **sintering**

permanent consolidation of a moulding body from a compacted powder aggregate material by means of a firing process, in which a decrease in the porosity, an increase in the density and a (sinter) shrinkage occur

Note 1 to entry: The temperature here shall be sufficiently high to cause densification but shall not be so high that a deformation of the moulding body occurs.

### 3.6

#### **sintered metal**

blanks produced from metal powder for milling via CAD/CAM technology for restorations made from base metal alloys, which are sintered in inert gas (argon) at temperatures of 1 200 °C to 1 400 °C

## **4 Measurement and test method**

### **4.1 General**

This document describes the calibration of resistance-heated high temperature sintering furnaces by means of a separate thermocouple. The furnaces shall be calibrated ex works in the same way for all manufacturers at a temperature of 1 500 °C. In addition, the deviation in the actual temperature at 1 000 °C shall be determined and a maximum permissible deviation specified.

### **4.2 Test devices and test equipment**

#### **4.2.1 Thermocouple fixture**

The thermocouple fixture shall be made from a lightweight material resistant to high temperatures that is white in colour. The thermocouple shall be set up corresponding to [Figure 1](#).

- a) material: polycrystalline ceramic fibres, for example, Al<sub>2</sub>O<sub>3</sub>: 75 % to 85 %; SiO<sub>2</sub>: 15 % to 25 %; about 400 kg/m<sup>3</sup>;
- b) height:  $X = (20 \pm 2)$  mm (depending on the furnace chamber);
- c) diameter:  $(40 \pm 2)$  mm (depending on the furnace chamber).

#### 4.2.2 Thermocouple

The thermocouple has the following specifications:

- a) thermocouple Pt10Rh-Pt (type S) according to IEC 60584-1:2013, with a limit deviation in the thermoelectric voltage of class 1 according to IEC 60584-1:2013, Table 12;


NOTE Pt13Rh-Pt (type R) according to IEC 60584-1:2013 is permissible as an alternative.

- b) diameter of the legs: 0,5 mm according to IEC 60584-3;
- c) diameter of the head:  $(1,5 \pm 0,5)$  mm;
- d) distance of the legs:  $(10 \pm 2)$  mm;
- e) height above the thermocouple fixture (depending on the furnace chamber, at the location of the object to be fired), for example,  $(10 \pm 2)$  mm.

The thermocouple shall be located centrally at a height  $Y = (10 \pm 2)$  mm above the object level (see [Figure 1](#)). The horizontal distance of the connecting wires protruding out of the thermocouple fixture is  $(10 \pm 2)$  mm.

Alternatively, the thermocouple can be introduced directly into the base.

Dimensions in millimetres

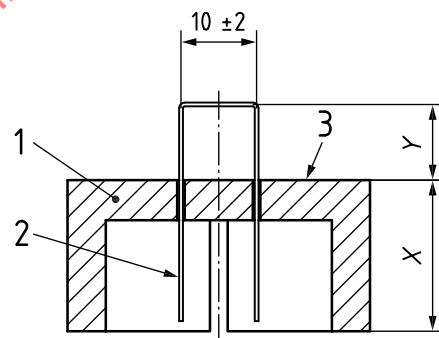

#### Key

- X height of the thermocouple fixture
- Y height of the thermocouple above the object level
- 1 thermocouple fixture
- 2 thermocouple
- 3 object level

**Figure 1 — Layout of the thermocouple on the thermocouple fixture**

#### 4.2.3 Compensating cable

The compensating cable for the thermocouple shall have a limiting deviation of the compensating cable of class 2 in accordance with IEC 60584-3. The connection point shall be compensated by the measuring device.

#### 4.2.4 Temperature indicating device

The temperature indicating device shall be calibrated to  $\pm 1,2$  °C between 400 °C and 1 550 °C (e.g. HP Data Logger or Ezecal<sup>1)</sup>).

#### 4.2.5 High temperature sintering furnace

### 4.3 Implementation

#### 4.3.1 Layout of the thermocouple

The thermocouple shall be installed centrally in the firing chamber of the high temperature sintering furnace or in the position where the firing material is located in accordance with the manufacturer's specifications.

#### 4.3.2 Heating phase

Before beginning the calibration, it shall be established that the high temperature sintering furnace is ready for operation.

The heating rate during the heating phase shall be minimum 10 °C/min. Calibration shall take place under ambient conditions (no negative pressure or vacuum).

#### 4.3.3 Test temperature 1

The high temperature sintering furnace shall be brought to a first test temperature of 1 000 °C.

#### 4.3.4 Holding time 1

The holding time begins when the display on the high temperature sintering furnace indicates that the set test temperature has been reached. The holding time is 10 min.

#### 4.3.5 First measurement

During the first holding time, the temperature values determined via the external thermocouple shall be read off and noted after 0 s, 15 s, 60 s, 120 s and 600 s.

#### 4.3.6 Test temperature 2

The high temperature sintering furnace shall be brought to a second temperature of 1 500 °C.

#### 4.3.7 Holding time 2

The holding time begins when the display on the high-temperature sintering furnace indicates that the set test temperature has been reached. The holding time is 10 min.

#### 4.3.8 Second measurement

During the second holding time, the temperature values determined via the external thermocouple shall be read off and noted after 0 s, 15 s, 60 s, 120 s and 600 s.

---

1) HP Data Logger and Ezecal are examples of suitable products available commercially. This information is given for the convenience of the users of this document and does not constitute an endorsement of this product by ISO.

#### 4.3.9 Interpretation

For both test temperatures, the relevant maximum deviation from the setpoint temperature as well as the mean deviation from the setpoint temperature (average value from the five measurements) shall be determined.

#### 4.3.10 Adjustment

If the measured temperatures deviate from the setpoint temperatures by more than 10 °C, the control electronics (display) shall be adjusted to the attained target-(nominal)-temperature.

If the sintering furnace has been adjusted, the test cycle shall then be repeated.

### 5 Test report

A test report shall be prepared. The test report shall include at least the following information:

- a) manufacturer and device type of the high-temperature sintering furnace;
- b) serial number of the high-temperature sintering furnace;
- c) test device, e.g. data logger;
- d) record with a setpoint/actual comparison at both test temperatures, as well as documentation of corresponding measures (adjustment);
- e) indication of the measured largest and mean deviations before the adjustment (only if testing after delivery to the user) and, if applicable, after the adjustment;
- f) all parameters defined in this document (heating rate, requirements for the measuring apparatus, type of thermocouple used, etc.) should be part of the test report as a pre-printed form;
- g) reference to this document, i.e. ISO 13078-3:2023;
- h) any deviations from the procedure;
- i) any unusual features observed;
- j) date of the test;
- k) name of the test laboratory or the identification number of the test technician if a calibration is conducted as part of the quality control.