

INTERNATIONAL ISO/IEEE STANDARD 11073-10404

Second edition
2022-12

Health informatics — Device interoperability —

Part 10404: Personal health device communication — Device specialization — Pulse oximeter

Informatique de santé — Interopérabilité des dispositifs —

*Partie 10404: Communication entre dispositifs de santé personnels —
Spécialisation des dispositifs — Oxymètre de pouls*



IEEE

Reference number
ISO/IEEE 11073-10404:2022(E)

© IEEE 2021



COPYRIGHT PROTECTED DOCUMENT

© IEEE 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from IEEE at the address below.

Institute of Electrical and Electronics Engineers, Inc
3 Park Avenue, New York
NY 10016-5997, USA

Email: stds.ipr@ieee.org
Website: www.ieee.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted (see www.iso.org/directives).

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

ISO/IEEE 11073-10404 was prepared by the *IEEE 11073 Standards Committee of the IEEE Engineering in Medicine and Biology Society* (as IEEE Std 11073-10404-2020) and drafted in accordance with its editorial rules. It was adopted, under the “fast-track procedure” defined in the Partner Standards Development Organization cooperation agreement between ISO and IEEE, by Technical Committee ISO/TC 215, *Health informatics*.

This second edition cancels and replaces the first edition (ISO/IEEE 11073-10404:2010), which has been technically revised.

A list of all parts in the ISO/IEEE 11073 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10404:2022

IEEE Std 11073-10404™-2020
(Revision of IEEE Std 11073-10404-2008)

Health informatics—Personal health device communication

Part 10404: Device specialization— Pulse oximeter

Developed by the
IEEE 11073™ Standards Committee
of the
IEEE Engineering in Medicine and Biology Society

Approved 30 January 2020
IEEE SA Standards Board

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10404:2022

Abstract: Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth pulse oximetry devices and compute engines (e.g., cell phones, personal computers, personal health appliances, set top boxes) in a manner that enables plug-and-play interoperability. It leverages appropriate portions of existing standards including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth pulse oximeters.

Keywords: IEEE 11073-10404™, medical device communication, personal health devices, PHD, pulse oximeter

The Institute of Electrical and Electronics Engineers, Inc.
3 Park Avenue, New York, NY 10016-5997, USA

Copyright © 2021 by The Institute of Electrical and Electronics Engineers, Inc.
All rights reserved. Published 7 January 2021. Printed in the United States of America.

IEEE is a registered trademark in the U.S. Patent & Trademark Office, owned by The Institute of Electrical and Electronics Engineers, Incorporated.

PDF: ISBN 978-1-5044-6458-1 STD24061
Print: ISBN 978-1-5044-6459-8 STDPD24061

IEEE prohibits discrimination, harassment, and bullying.

For more information, visit <https://www.ieee.org/about/corporate/governance/p9-26.html>.

No part of this publication may be reproduced in any form, in an electronic retrieval system or otherwise, without the prior written permission of the publisher.

Important Notices and Disclaimers Concerning IEEE Standards Documents

IEEE Standards documents are made available for use subject to important notices and legal disclaimers. These notices and disclaimers, or a reference to this page (<https://standards.ieee.org/ipr/disclaimers.html>), appear in all standards and may be found under the heading “Important Notices and Disclaimers Concerning IEEE Standards Documents.”

Notice and Disclaimer of Liability Concerning the Use of IEEE Standards Documents

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE SA) Standards Board. IEEE develops its standards through an accredited consensus development process, which brings together volunteers representing varied viewpoints and interests to achieve the final product. IEEE Standards are documents developed by volunteers with scientific, academic, and industry-based expertise in technical working groups. Volunteers are not necessarily members of IEEE or IEEE SA, and participate without compensation from IEEE. While IEEE administers the process and establishes rules to promote fairness in the consensus development process, IEEE does not independently evaluate, test, or verify the accuracy of any of the information or the soundness of any judgments contained in its standards.

IEEE makes no warranties or representations concerning its standards, and expressly disclaims all warranties, express or implied, concerning this standard, including but not limited to the warranties of merchantability, fitness for a particular purpose and non-infringement. In addition, IEEE does not warrant or represent that the use of the material contained in its standards is free from patent infringement. IEEE standards documents are supplied “AS IS” and “WITH ALL FAULTS.”

Use of an IEEE standard is wholly voluntary. The existence of an IEEE Standard does not imply that there are no other ways to produce, test, measure, purchase, market, or provide other goods and services related to the scope of the IEEE standard. Furthermore, the viewpoint expressed at the time a standard is approved and issued is subject to change brought about through developments in the state of the art and comments received from users of the standard.

In publishing and making its standards available, IEEE is not suggesting or rendering professional or other services for, or on behalf of, any person or entity, nor is IEEE undertaking to perform any duty owed by any other person or entity to another. Any person utilizing any IEEE Standards document, should rely upon his or her own independent judgment in the exercise of reasonable care in any given circumstances or, as appropriate, seek the advice of a competent professional in determining the appropriateness of a given IEEE standard.

IN NO EVENT SHALL IEEE BE LIABLE FOR ANY DIRECT, INDIRECT, INCIDENTAL, SPECIAL, EXEMPLARY, OR CONSEQUENTIAL DAMAGES (INCLUDING, BUT NOT LIMITED TO: THE NEED TO PROCURE SUBSTITUTE GOODS OR SERVICES; LOSS OF USE, DATA, OR PROFITS; OR BUSINESS INTERRUPTION) HOWEVER CAUSED AND ON ANY THEORY OF LIABILITY, WHETHER IN CONTRACT, STRICT LIABILITY, OR TORT (INCLUDING NEGLIGENCE OR OTHERWISE) ARISING IN ANY WAY OUT OF THE PUBLICATION, USE OF, OR RELIANCE UPON ANY STANDARD, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGE AND REGARDLESS OF WHETHER SUCH DAMAGE WAS FORESEEABLE.

Translations

The IEEE consensus development process involves the review of documents in English only. In the event that an IEEE standard is translated, only the English version published by IEEE is the approved IEEE standard.

Official statements

A statement, written or oral, that is not processed in accordance with the IEEE SA Standards Board Operations Manual shall not be considered or inferred to be the official position of IEEE or any of its committees and shall not be considered to be, nor be relied upon as, a formal position of IEEE. At lectures, symposia, seminars, or educational courses, an individual presenting information on IEEE standards shall make it clear that the presenter's views should be considered the personal views of that individual rather than the formal position of IEEE, IEEE SA, the Standards Committee, or the Working Group.

Comments on standards

Comments for revision of IEEE Standards documents are welcome from any interested party, regardless of membership affiliation with IEEE or IEEE SA. However, **IEEE does not provide interpretations, consulting information, or advice pertaining to IEEE Standards documents.**

Suggestions for changes in documents should be in the form of a proposed change of text, together with appropriate supporting comments. Since IEEE standards represent a consensus of concerned interests, it is important that any responses to comments and questions also receive the concurrence of a balance of interests. For this reason, IEEE and the members of its Societies and Standards Coordinating Committees are not able to provide an instant response to comments, or questions except in those cases where the matter has previously been addressed. For the same reason, IEEE does not respond to interpretation requests. Any person who would like to participate in evaluating comments or in revisions to an IEEE standard is welcome to join the relevant IEEE working group. You can indicate interest in a working group using the Interests tab in the Manage Profile & Interests area of the [IEEE SA myProject system](#). An IEEE Account is needed to access the application.

Comments on standards should be submitted using the [Contact Us](#) form.

Laws and regulations

Users of IEEE Standards documents should consult all applicable laws and regulations. Compliance with the provisions of any IEEE Standards document does not constitute compliance to any applicable regulatory requirements. Implementers of the standard are responsible for observing or referring to the applicable regulatory requirements. IEEE does not, by the publication of its standards, intend to urge action that is not in compliance with applicable laws, and these documents may not be construed as doing so.

Data privacy

Users of IEEE Standards documents should evaluate the standards for considerations of data privacy and data ownership in the context of assessing and using the standards in compliance with applicable laws and regulations.

Copyrights

IEEE draft and approved standards are copyrighted by IEEE under US and international copyright laws. They are made available by IEEE and are adopted for a wide variety of both public and private uses. These include both use, by reference, in laws and regulations, and use in private self-regulation, standardization, and the promotion of engineering practices and methods. By making these documents available for use and adoption by public authorities and private users, IEEE does not waive any rights in copyright to the documents.

Photocopies

Subject to payment of the appropriate licensing fees, IEEE will grant users a limited, non-exclusive license to photocopy portions of any individual standard for company or organizational internal use or individual, non-commercial use only. To arrange for payment of licensing fees, please contact Copyright Clearance Center, Customer Service, 222 Rosewood Drive, Danvers, MA 01923 USA; +1 978 750 8400; <https://www.copyright.com/>. Permission to photocopy portions of any individual standard for educational classroom use can also be obtained through the Copyright Clearance Center.

Updating of IEEE Standards documents

Users of IEEE Standards documents should be aware that these documents may be superseded at any time by the issuance of new editions or may be amended from time to time through the issuance of amendments, corrigenda, or errata. An official IEEE document at any point in time consists of the current edition of the document together with any amendments, corrigenda, or errata then in effect.

Every IEEE standard is subjected to review at least every 10 years. When a document is more than 10 years old and has not undergone a revision process, it is reasonable to conclude that its contents, although still of some value, do not wholly reflect the present state of the art. Users are cautioned to check to determine that they have the latest edition of any IEEE standard.

In order to determine whether a given document is the current edition and whether it has been amended through the issuance of amendments, corrigenda, or errata, visit [IEEE Xplore](#) or [contact IEEE](#). For more information about the IEEE SA or IEEE's standards development process, visit the IEEE SA Website.

Errata

Errata, if any, for all IEEE standards can be accessed on the [IEEE SA Website](#). Search for standard number and year of approval to access the web page of the published standard. Errata links are located under the Additional Resources Details section. Errata are also available in [IEEE Xplore](#). Users are encouraged to periodically check for errata.

Patents

IEEE Standards are developed in compliance with the [IEEE SA Patent Policy](#).

Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken by the IEEE with respect to the existence or validity of any patent rights in connection therewith. If a patent holder or patent applicant has filed a statement of assurance via an Accepted Letter of Assurance, then the statement is listed on the IEEE SA Website at <https://standards.ieee.org/about/sasb/patcom/patents.html>. Letters of Assurance may indicate whether the Submitter is willing or unwilling to grant licenses under patent rights without compensation or under reasonable rates, with reasonable terms and conditions that are demonstrably free of any unfair discrimination to applicants desiring to obtain such licenses.

Essential Patent Claims may exist for which a Letter of Assurance has not been received. The IEEE is not responsible for identifying Essential Patent Claims for which a license may be required, for conducting inquiries into the legal validity or scope of Patents Claims, or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from the IEEE Standards Association.

IMPORTANT NOTICE

IEEE Standards do not guarantee or ensure safety, security, health, or environmental protection, or ensure against interference with or from other devices or networks. IEEE Standards development activities consider research and information presented to the standards development group in developing any safety recommendations. Other information about safety practices, changes in technology or technology implementation, or impact by peripheral systems also may be pertinent to safety considerations during implementation of the standard. Implementers and users of IEEE Standards documents are responsible for determining and complying with all appropriate safety, security, environmental, health, and interference protection practices and all applicable laws and regulations.

Participants

At the time this standard was completed, the Personal Health Devices Working Group had the following membership:

Daidi Zhong, Co-Chair
Michael J. Kirwan, Co-Chair

Karsten Aalders
 Charles R. Abbruscato
 Nabil Abujbara
 Maher Abuzaid
 James Agnew
 Manfred Aigner
 Jorge Alberola
 David Aparisi
 Lawrence Arne
 Diego B. Arquillo
 Serafin Arroyo
 Muhammad Asim
 Kit August
 Doug Baird
 David Baker
 Anindya Bakshi
 Abira Balanadarasan
 Ananth Balasubramanian
 Sunlee Bang
 M. Jonathan Barkley
 Gilberto Barrón
 David Bean
 John Bell
 Olivia Bellamou-Huet
 Rudy Belliardi
 Kathryn M. Bennett
 Daniel Bernstein
 George A. Bertos
 Chris Biernacki
 Ola Björnsne
 Thomas Blackadar
 Marc Blanchet
 Thomas Bluethner
 Douglas P. Bogia
 Xavier Boniface
 Shannon Boucousis
 Julius Broma
 Lyle G. Bullock, Jr.
 Bernard Burg
 Chris Burns
 Jeremy Byford-Rew
 Satya Calloji
 Xiaoying Cao
 Carole C. Carey
 Craig Carlson
 Santiago Carot-Nemesio
 Randy W. Carroll
 Simon Carter
 Seungchul Chae
 Rahul Chauhan
 Peggy Chien
 David Chiu
 Jinyong Choi

Chia-Chin Chong
 Saeed A. Choudhary
 Jinhan Chung
 John A. Cogan
 John T. Collins
 Cory Condek
 Todd H. Cooper
 David Cornejo
 Douglas Coup
 Nigel Cox
 Hans Crommenacker
 Tomio Crosley
 Allen Curtis
 Jesús Daniel Trigo
 David Davenport
 Russell Davis
 Sushil K. Deka
 Ciro de la Vega
 Pedro de-las-Heras-Quiros
 Jim Dello Stritto
 Kent Dicks
 Hyoungdo Do
 Jonathan Dougherty
 Xiaolian Duan
 Sourav Dutta
 Jakob Ehrensverd
 Fredrik Einberg
 Javier Escayola Calvo
 Mark Estes
 Leonardo Estevez
 Hailing Feng
 Bosco T. Fernandes
 Christoph Fischer
 Morten Flintrup
 Joseph W. Forler
 Russell Foster
 Eric Freudenthal
 Matthias Frohner
 Ken Fuchs
 Jing Gao
 Qi Gao
 Marcus Garbe
 John Garguilo
 Rick Geimer
 Igor Gejdos
 Ferenc Gerbovics
 Alan Godfrey
 Nicolae Goga
 Julian Goldman
 Raul Gonzalez Gomez
 Chris Gough
 Channa Gowda
 Charles M. Gropper

Amit Gupta
 Jeff Guttmacher
 Rasmus Haahr
 Christian Habermann
 Michael Hagerty
 Jerry Hahn
 Robert Hall
 Shu Han
 Nathaniel Hamming
 Rickey L. Hampton
 Sten Hanke
 Aki Harma
 Jordan Hartmann
 Kai Hassing
 Avi Hauser
 Wolfgang Heck
 Nathaniel Heintzman
 Charles Henderson
 Jun-Ho Her
 Helen B. Hernandez
 Timothy L. Hirou
 Allen Hobbs
 Alex Holland
 Arto Holopainen
 Kris Holtzclaw
 Xinyi Hong
 Robert Hoy
 Di Hu
 Anne Huang
 Zhiqiang Huang
 Zhiyong Huang
 Ron Huby
 David Hughes
 Robert D. Hughes
 Jiyoung Huh
 Hugh Hunter
 Philip O. Isaacson
 Atsushi Ito
 Michael Jaffe
 Praduman Jain
 Danny Jochelson
 Akiyoshi Kabe
 Steve Kahle
 Tomio Kamioka
 James J. Kang
 Kei Kariya
 Andy Kaschl
 Junzo Kashiara
 Colin Kennedy
 Ralph Kent
 Laurie M. Kermes
 Ahmad Kheirandish
 Junhyung Kim

Minho Kim	Yoshiteru Nozoe	Nicholas Steblay
Min-Joon Kim	Abraham Ofek	Lars Steubesand
Taekon Kim	Brett Olive	John (Ivo) Stivorice
Tetsuya Kimura	Begonya Ota	Raymond A. Strickland
Michael J. Kirwan	Marco Paleari	Chandrasekaran Subramaniam
Alfred Kloos	Bud Panjwani	Hermann Suominen
Jeongmee Koh	Carl Pantiskas	Lee Surprenant
Jean-Marc Koller	Harry P. Pappas	Ravi Swami
John Koon	Hanna Park	Ray Sweidan
Patty Krantz	Jong-Tae Park	Na Tang
Raymond Krasinski	Myungeun Park	Yi Tang
Alexander Kraus	Soojun Park	Haruyuyki Tatsumi
Ramesh Krishna	Phillip E. Pash	Isabel Tejero
Geoffrey Kruse	Tong Bi Pei	Tom Thompson
Falko Kuester	Soren Petersen	Jonas Tirén
Rafael Lajara	James Petisce	Janet Traub
Pierre Landau	Peter Piction	Gary Tschautscher
Jaechul Lee	Michael Pliskin	Masato Tsuchida
JongMuk Lee	Varshney Prabodh	Ken Tubman
Kyong Ho Lee	Jeff Price	Akib Uddin
Rami Lee	Harald Prinzhorn	Sumi Unadkat
Sungkee Lee	Harry Qiu	Fabio Urbani
Woojae Lee	Tanzilur Rahman	Philipp Urbauer
Qiong Li	Phillip Raymond	Laura Vanzago
Xiangchen Li	Terrie Reed	Alpo Värri
Yingsong Li	Barry Reinhold	Andrei Vasilateanu
Zhuofang Li	Brian Reinhold	Dalimar Velez
Patrick Lichter	Melvin I. Reynolds	Martha Velez
Lin Lin	John G. Rhoads	Rudi Voon
Jisoon Lim	Jeffrey S. Robbins	Barry Vornbrock
Joon-Ho Lim	Chris Roberts	Isobel Walker
Liang Liu	Moskowitz Robert	David Wang
Xiaoming Liu	Stefan Robert	Linling Wang
Wei-Jung Lo	Scott M. Robertson	Jerry P. Wang
Charles Lowe	Timothy Robertson	Yao Wang
Don Ludolph	Patricia Roder	Yi Wang
Christian Lusztick	David Rosales	Steve Warren
Bob MacWilliams	Bill Saltzstein	Fujio Watanabe
Srikanth Madhurbootheswaran	Giovanna Sannino	Toru Watsuji
Miriam L. Makhoul	Jose A. Santos-Cadenas	David Weissman
Romain Marmot	Stefan Sauermann	Kathleen Wible
Sandra Martinez	John Sawyer	Paul Williamson
Miguel Martínez de	Alois Schloegl	Jan Wittenber
Espronceda Cámara	Paul S. Schluter	Jia-Rong Wu
Peter Mayhew	Mark G. Schnell	Will Wykeham
Jim McCain	Richard A. Schrenker	Ariton Xhafa
László Meleg	Antonio Scorpiniti	Ricky Yang
Alexander Mense	KwangSeok Seo	Shaoqin Ye
Behnaz Minaei	Riccardo Serafin	Melanie S. Yeung
Jinsei Miyazaki	Sid Shaw	Qiang Yin
Erik Moll	Frank Shen	Done-Sik Yoo
Dan Moore	Min Shih	Zhi Yu
Carsten Mueglitz	Mazen Shihabi	Jianchao Zeng
Soundharya Nagasubramanian	Redmond Shouldice	Jason Zhang
Alex Neefus	Sternly K. Simon	Jie Zhao
Trong-Nghia Nguyen-Dobinsky	Marjorie Skubic	Thomas Zhao
Michael E. Nidd	Robert Smith	Daidi Zhong
Jim Niswander	Ivan Soh	Hongyuan Zhong
Hongliang Niu	Motoki Sone	Yuanhong Zhong
Hiroaki Niwamoto	Emily Sopensky	Miha Zoubek
Thomas Norgall	Rajagopalan Srinivasan	Szymon Zyskoter

The following members of the individual balloting committee voted on this standard. Balloters may have voted for approval, disapproval, or abstention.

Bjoern Andersen
Lyle Bullock
Keith Chow
Malcolm Clarke
Kenneth Fuchs
David Fuschi
Randall Groves
Robert Heile

Werner Hoelzl
Noriyuki Ikeuchi
Atsushi Ito
Raj Jain
Piotr Karocki
Martin Kasparick
Raymond Krasinski
H. Moll

Iulian Profir
Beth Pumo
Stefan Schlichting
Janek Schumann
Walter Struppler
Oren Yuen
Janusz Zalewski
Daidi Zhong

When the IEEE SA Standards Board approved this standard on 30 January 2020, it had the following membership:

Gary Hoffman, Chair
Vacant Position, Vice Chair
Jean-Philippe Faure, Past Chair
Konstantinos Karachalios, Secretary

Ted Burse
Doug Edwards
J. Travis Griffith
Grace Gu
Guido R. Hiertz
Joseph L. Koepfinger*
John D. Kulick

David J. Law
Howard Li
Dong Liu
Kevin Lu
Paul Nikolich
Damir Novosel
Jon Walter Rosdahl

Dorothy Stanley
Mehmet Ulema
Lei Wang
Sha Wei
Philip B. Winston
Daidi Zhong
Jingyi Zhou

*Member Emeritus

Introduction

This introduction is not part of IEEE Std 11073-10404-2020, Health informatics—Personal health device communication—Part 10404: Device specialization—Pulse oximeter.

ISO/IEEE 11073 standards enable communication between medical devices and external computer systems. This document uses the optimized framework created in IEEE Std 11073-20601-2019TM and describes a specific, interoperable communication approach for the pulse oximeter.¹ These standards align with, and draw on, the existing clinically focused standards to provide support for communication of data from clinical or personal health devices.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10404:2022

¹ Information on references can be found in Clause 2.

Contents

1. Overview	12
1.1 Scope	12
1.2 Purpose	12
1.3 Context	12
2. Normative references.....	13
3. Definitions, acronyms, and abbreviations	13
3.1 Definitions	13
3.2 Acronyms and abbreviations	14
4. Introduction to ISO/IEEE 11073 personal health devices	14
4.1 General	14
4.2 Introduction to IEEE 11073-20601 modeling constructs.....	15
4.3 Compliance with other standards.....	15
5. Pulse oximeter device concepts and modalities.....	16
5.1 General	16
5.2 Device types	16
5.3 General concepts.....	16
5.4 Collected data	17
5.5 Derived data.....	19
5.6 Stored data.....	19
5.7 Device configurations.....	19
6. Pulse oximeter DIM	20
6.1 Overview	20
6.2 Class extensions.....	20
6.3 Object instance diagram	20
6.4 Types of configuration.....	21
6.5 MDS object.....	22
6.6 Numeric objects.....	26
6.7 Real-time sample array (RT-SA) objects.....	36
6.8 Enumeration objects	37
6.9 PM-store objects.....	41
6.10 Scanner objects.....	45
6.11 Class extension objects.....	48
6.12 Pulse oximeter information model extensibility rules	48
7. Pulse oximeter service model.....	48
7.1 General	48
7.2 Object access services.....	48
7.3 Object access EVENT REPORT services	52
8. Pulse oximeter communication model.....	52
8.1 Overview	52
8.2 Communications characteristics	52
8.3 Association procedure	53
8.4 Configuring procedure.....	55
8.5 Operating procedure	56
8.6 Time synchronization	57

9. Test associations	57
9.1 Behavior with standard configuration.....	57
9.2 Behavior with extended configurations	58
10. Conformance	58
10.1 Applicability	58
10.2 Conformance specification	58
10.3 Levels of conformance	58
10.4 Implementation conformance statements (ICSs)	59
Annex A (informative) Bibliography	63
Annex B (normative) Additional ASN.1 definitions	64
Annex C (normative) Allocation of identifiers	65
Annex D (informative) Message sequence examples	67
Annex E (informative) PDU examples.....	69
Annex F (informative) Revision history.....	81

Health informatics—Personal health device communication

Part 10404: Device specialization— Pulse oximeter

1. Overview

1.1 Scope

Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth pulse oximeter devices and compute engines (e.g., cell phones, personal computers, personal health appliances, set top boxes) in a manner that enables plug-and-play (PnP) interoperability. It leverages appropriate portions of existing standards including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth pulse oximeters.

1.2 Purpose

This standard addresses a need for an openly defined, independent standard for controlling information exchange to and from personal health devices (PHDs) and compute engines (e.g., cell phones, personal computers, personal health appliances, set top boxes). Interoperability is key to growing the potential market for these devices and enabling people to be better informed participants in the management of their health.

1.3 Context

See IEEE Std 11073-20601-2019^{TM2} for an overview of the environment within which this standard is written.

This standard, IEEE Std 11073-10404, defines the device specialization for the pulse oximeter, being a specific agent type, and provides a description of the device concepts, its capabilities, and its implementation according to this standard.

This standard is based on IEEE Std 11073-20601-2019, which in turn draws information from both ISO/IEEE 11073-10201:2004 [B6]³ and ISO/IEEE 11073-20101:2004 [B7]. The medical device encoding rules (MDER) used within this standard are fully described in IEEE Std 11073-20601-2019.

² Information on references can be found in Clause 2.

³ The numbers in brackets correspond to the numbers in the bibliography in Annex A.

This standard defines specialized nomenclature codes that will be collected in IEEE Std 11073-10101-2019TM. Between this standard, IEEE Std 11073-10101-2019, IEEE Std 11073-20601-2019 and other IEEE Std 11073-104xx, all required nomenclature codes for implementation are documented. New codes may be defined in newer versions / revisions of each of these documents. In the case of a conflict, where one term code has been assigned to two separate semantic concepts with different RefIDs, in general the oldest definition that is in actual use should take precedence. The same policy applies when one RefID has two different code values assigned in different specifications. The resolution of such conflicts will be determined through joint action by the responsible work groups and other stakeholders and any corrective action published as corrigenda.

NOTE—In this standard, ISO/IEEE P11073-104zz is used to refer to the collection of device specialization standards that utilize IEEE Std 11073-20601-2019, where zz can be any number from 01 to 99, inclusive.⁴

2. Normative references

The following referenced documents are indispensable for the application of this document (i.e., they must be understood and used, so that each referenced document is cited in text and its relationship to this document is explained). For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments or corrigenda) applies.

IEEE Std 11073-20601-2019, Health informatics—Personal health device communication—Part 20601: Application profile—Optimized Exchange Protocol.^{5, 6}

IEEE Std 11073-10101-2019, Health informatics—Point-of-care medical device communication—Part 10101: Nomenclature.

See Annex A for all informative material referenced by this standard.

3. Definitions, acronyms, and abbreviations

3.1 Definitions

For the purposes of this standard, the following terms and definitions apply. The *IEEE Standards Dictionary Online* [B1] should be referenced for terms not defined in this clause.⁷

agent: A node that collects and transmits personal health data to an associated manager.

class: In object-oriented modeling, a class describes the attributes, methods, and events that objects instantiated from the class utilize.

compute engine: See: **manager**.

device: A physical apparatus implementing either an agent or manager role.

handle: An unsigned 16-bit number that is locally unique and identifies one of the object instances within an agent.

⁴ Notes in text, tables, and figures are given for information only and do not contain requirements needed to implement the standard.

⁵ IEEE publications are available from The Institute of Electrical and Electronics Engineers (<https://standards.ieee.org/>).

⁶ The IEEE standards or products referred to in Clause 2 are trademarks owned by The Institute of Electrical and Electronics Engineers, Incorporated.

⁷ *IEEE Standards Dictionary Online* is available at: <http://dictionary.ieee.org>. An IEEE Account is required for access to the dictionary, and one can be created at no charge on the dictionary sign-in page.

manager: A node receiving data from one or more associated agent systems. Examples of managers include a cellular phone, health appliance, set top box, or a computer system.

object: In object-oriented modeling, a particular instantiation of a class. The instantiation realizes attributes, methods, and events from the class.

obj-handle: *See:* **handle**.

personal health device: A device used in personal health applications.

personal telehealth device: *See:* **personal health device**.

photoplethysmographic waveform: *See:* **plethysmogram**.

plethysmogram: Sequence of samples related to the sequential time-varying light absorption due to effects of pulsatile blood flow.

plethysmographic: *See:* **plethysmogram**.

SpO₂: Percentage oxygen saturation of haemoglobin as measured by a pulse oximeter, where this measurement is an estimate of the fraction of functional haemoglobin (or hemoglobin) in arterial blood that is saturated with oxygen.

NOTE—For more information about SpO₂, see ISO 80601-2-61:2017 [B9].

3.2 Acronyms and abbreviations

APDU	application protocol data unit
ASN.1	Abstract Syntax Notation One
DIM	domain information model
EUI-64	extended unique identifier (64 bits)
ICS	implementation conformance statement
ID	identifier
MDC	medical device communication
MDER	medical device encoding rules
MDS	medical device system
MOC	managed object class
OID	object identifier
PDU	protocol data unit
PHD	personal health device
RT-SA	real-time sample array
SpO ₂	percentage oxygen saturation of haemoglobin
VMO	virtual medical object

4 Introduction to ISO/IEEE 11073 personal health devices

4.1 General

This standard and the remainder of the series of ISO/IEEE 11073 personal health device (PHD) standards fit in the larger context of the ISO/IEEE 11073 series of standards. The full suite of standards enables agents to interconnect and interoperate with both managers and computerized healthcare information systems. See IEEE Std 11073-20601-2019 for a description of the guiding principles for this series of ISO/IEEE 11073 Personal Health Device standards.

IEEE Std 11073-20601-2019 supports the modeling and implementation of an extensive set of personal health devices. This standard defines aspects of the pulse oximeter device. It describes all aspects necessary to implement the application layer services and data exchange protocol between an ISO/IEEE 11073 PHD pulse oximetry agent and a manager. This standard defines a subset of the objects and functionality contained in IEEE Std 11073-20601-2019, extending and adding definitions where appropriate.

All nomenclature codes referenced in this standard are collected in Annex C. Annex C may contain definitions of codes that are used by this standard and that are not yet present in the referenced versions of IEEE Std 11073-10101-2019 and IEEE Std 11073-20601-2019.

4.2 Introduction to IEEE 11073-20601 modeling constructs

4.2.1 General

The ISO/IEEE 11073 series of standards, and in particular IEEE Std 11073-20601-2019, is based on an object-oriented systems management paradigm. The overall system model is divided into three principal components: the domain information model (DIM), the service model, and the communication model. See IEEE Std 11073-20601-2019 for a detailed description of the modeling constructs.

4.2.2 Domain information model (DIM)

The DIM is a hierarchical model that describes an agent as a set of objects. These objects and their attributes represent the elements that control behavior and report on the status of the agent and data that an agent can communicate to a manager. Communication between the agent and manager is defined by the application protocol in IEEE Std 11073-20601-2019.

4.2.3 Service model

The service model defines the conceptual mechanisms for the data exchange services. Such services are mapped to messages that are exchanged between the agent and manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. The messages defined in IEEE Std 11073-20601-2019 can coexist with messages defined in other standard application profiles defined in the ISO/IEEE 11073 series of standards.

4.2.4 Communication model

In general, the communication model supports the topology of one or more agents communicating over logical point-to-point connections to a single manager. For each logical point-to-point connection, the dynamic system behavior is defined by a connection state machine as specified in IEEE Std 11073-20601-2019.

4.2.5 Implementing the models

An agent implementing this standard shall implement all mandatory elements of the information, service, and communication models as well as all conditional elements where the condition is met. The agent should implement the recommended elements, and it may implement any combination of the optional elements. A manager implementing this standard shall utilize at least one of the mandatory, conditional, recommended, or optional elements. In this context, “utilize” means to use the element as part of the primary function of the manager device. For example, a manager whose primary function is to display data would need to display a piece of data in the element in order to utilize it.

4.3 Compliance with other standards

Devices that comply with this standard may also be required to comply with other domain- and device-specific standards that supersede the requirements of this standard with respect to issues including safety,

reliability, and risk management. A user of this standard is expected to be familiar with all other such standards that apply and to comply with any higher specifications thus imposed.

Typically, medical devices should comply with the IEC 60601-1 [B2] base standards with respect to electrical and mechanical safety and any device-specific standard as might be defined in the IEC 60601-2 [B3] series of standards. Software aspects may apply through standards such as IEC 62304/EN 62304 [B4]. Devices that comply with this standard implement higher layers of network software and utilize lower layers as appropriate to the application. The requirements on performance of such applications and conformance are defined elsewhere and are outside the scope of this standard. Moreover, the use of any medical equipment is subject to risk assessment and risk management appropriate to the application. Some relevant examples are ISO 14971:2007 [B8] and IEC 80001-1 [B5]. The requirements of such risk assessment, risk management, and conformance are outside the scope of this standard. The applicable versions of the referenced safety related standards may differ per country.

5. Pulse oximeter device concepts and modalities

5.1 General

This clause presents the general concepts of pulse oximeter equipment. In the context of PHDs in the ISO/IEEE 11073 family of standards, a pulse oximeter, also called an oximeter, provides a noninvasive estimate of functional oxygen of arterial haemoglobin (SpO_2) from a light signal interacting with tissue, by using the time-dependent changes in tissue optical properties that occur with pulsatile blood flow (see Draft Guidance for Industry and FDA Staff **Error! Reference source not found.**). Applying the Beer-Lambert law of light absorption through such an arterial network, the fraction of oxygenation of arterial haemoglobin can be estimated. This estimate, normally expressed as a percentage by multiplying that fraction by 100, is known as SpO_2 . Occasionally, this estimate may be referenced as $\%\text{SpO}_2$. ISO 80601-2-61:2017 [B9] contains additional information applicable to pulse oximetry.

5.2 Device types

Pulse oximeter systems with applicability in the personal health space may take on a variety of configurations and sensor compositions, and their configurations have suitability in different personal health application spaces. Pulse oximeter equipment comprises a pulse oximeter monitor, a pulse oximeter probe, and a probe cable extender, if provided. Some oximeters are all-in-one assemblies, where the optical probe, processing, and display components are in a single package. Other oximeters may consist of separate sensor and processing/display components. Still others may place the sensor and signal processing in one component, and send that information into an external component for display and storage. Pulse oximeters may place sensors in numerous locations on the body and use transconductance and reflectance of the light path. This standard assumes all measurements are equal and provides a single measure with no differentiation of location. In addition, other configurations may add storage capability into the system. This implies that different information models may be best suited for each particular device configuration.

5.3 General concepts

5.3.1 Noninvasive measurement

The scope of this specialization covers the intended use of pulse oximeter equipment, which includes, but is not limited to, the estimation of arterial oxygen haemoglobin saturation and pulse rate. This standard is not applicable to pulse oximeter equipment intended for use in laboratory research applications or to oximeters that require a blood sample (see ISO 80601-2-61:2017 [B9]). This standard does not cover measurement of oxygenation via blood extraction. This standard is not applicable to pulse oximeter equipment solely intended for foetal use.

The sensing mechanism may use either transmissive or reflective methods to measure blood oxygenation.

In addition, blood oxygenation is usually determined as a ratio of the absorbance of two different wavelengths of light, although more wavelengths may be used.

5.3.2 Acquisition modes

5.3.2.1 General

Pulse oximeters are used to measure SpO_2 within a variety of use scenarios.

5.3.2.2 Spot-check

In a spot-check scenario, a user may simply want to take a single, fully processed reading for transmission to a manager. For example, the user would attach the oximeter, whereupon the agent would take an oximetry and pulse rate reading. The agent would then begin communication with a manager and send that single reading. The manager may acknowledge the transmission so the agent can subsequently disassociate and return to its prior state.

5.3.2.3 Continuous monitoring

A continuous monitoring situation involves the pulse oximeter device measuring the user's oxygenation for some period of time greater than that needed to acquire a single measurement. Multiple measurements may be taken to acquire trending information.

5.3.2.4 Stored-and-forwarded measurements

Stored-and-forwarded measurements could be considered as a specialized, continuous monitoring application where the pulse oximetry device is not always in communication with a manager, and the oximeter records data over several minutes or hours. In this case, oximetry data are stored in the device for the duration of the study session and subsequently transferred to the manager at an appropriate time. This measurement communication style is distinct from the situation where temporarily stored measurements are transferred when the communication link is restored.

5.4 Collected data

5.4.1 General

This subclause describes the nature of the data that have been collected based on the acquisition modes described in 5.3.2.

5.4.2 Percentage of arterial haemoglobin oxygen saturation

5.4.2.1 SpO_2

Every oximeter sends at least one expression of SpO_2 . This is the primary measurement of a pulse oximeter. It is important to note that this measurement is determined through various signal processing techniques and can be expressed in different ways. Each method and expression has its applicability in particular application spaces (e.g., vital signs monitoring and diagnostic sleep studies). Often the reported SpO_2 has been processed with a variety of techniques in order to present the data for use in a number of ways.

In response to the various physiological phenomena and situations, SpO_2 measurements may be expressed in a variety of ways. Additional modalities for expressing SpO_2 are often used that are better suited to expose or suppress various physiological or environmental phenomena, as seen in 5.4.2.2. The following subclause outlines three expressions of SpO_2 that may be used by a device manufacturer to convey blood oxygenation level.

It is also conceivable that pulse oximeter equipment may deliver a single SpO_2 that is determined by one of these modalities. Furthermore, several of these distinct expressions may be transmitted concurrently during a measurement session. The manager, upon receiving this collection of information, may choose to display another subset of these expressions. It is required for a pulse oximeter agent to support at least one instance of this measurement.

5.4.2.2 Alternative expressions of SpO_2

One case of SpO_2 measurement involves a user wearing a sensor during unintentional or moderate activity. The result of this activity may be intermittent loss of signal acquisition. The most common expression of SpO_2 may be too sensitive to these effects and could result in a fluctuating (and, therefore, misleading) reading. An SpO_2 measurement modality known as “slow-response” modality has a characteristic that “smooths out” a series of measurements in some fashion, perhaps by changing an averaging parameter or by employing a different algorithm. This modality is defined in this standard.

During a sleep study, an apnea event results in a rapid desaturation of blood oxygenation. This SpO_2 measurement can be expressed by a “fast-response” modality that uses a technique that more effectively captures such events. The technique may vary among device manufacturers, but a distinct expression able to capture these rapid changes is defined in this standard.

The terms *slow-response* and *fast-response* are relative to a particular implementation and are not intended to show a comparison across devices or vendors. Note that these are descriptive terms intentionally left unspecific to allow more flexible interpretations within a particular implementation.

A pulse oximeter will often send SpO_2 measurements periodically; e.g., once every second. In addition, pulse oximeters may begin outputting measurements as soon as it has a reasonable estimate of functional haemoglobin oxygenation. Subsequent measurements may, in some fashion, converge on the oximeter’s best estimate. An additional modality, the “spot-check” modality, fulfills the desire to be able to perform and display a single SpO_2 measurement that is also its best estimate of functional haemoglobin oxygenation. In other words, a spot-check is not simply the first measurement, but the first *best* measurement. The specific manner in which this measurement is produced is specific to the pulse oximeter implementation. Once that measurement is transmitted, the measurement session is complete.

5.4.3 Pulse rate

The heart rate measured by a pulse oximeter is produced by a heartbeat, but also requires ejection of blood by the heart and generation of an arterial and tissue pressure wave that is detectable by photoplethysmographic means. Therefore, the pulse rate may be a less reliable measure of heart rate than that of directly measuring by electrocardiograph (ECG). As described in 5.4.2.1 and 5.4.2.2, the reported value or values may be determined in a variety of ways, and corresponding modalities of “slow-response,” “fast-response,” and “spot-check” are defined for pulse rate measurements. It is required for a pulse oximeter agent to support at least one instance of this feature.

5.4.4 Pulsatile occurrence

If a precisely timestamped occurrence of a pulse is transmitted to a manager, that information can be used in conjunction with other reported physiological events to derive another physiological measurement. Other application spaces may wish to indicate pulsatile occurrence with less precision for purposes of displaying, for instance, a flashing heart icon. It is not required for a pulse oximeter agent to support this feature.

5.4.5 Plethysmogram

There are applications where it is desired to visualize the sequence of samples related to the time-varying light absorption due to the effects of pulsatile blood flow. Often these samples are taken from a single wavelength light source, usually the wavelength less affected by changes in oxygen saturation. It is not required for a pulse oximeter agent to support this feature.

5.4.6 Pulsatile quality and signal characterization

Pulse oximeter manufacturers have many ways to characterize the quality of the pulsatile wave. Unfortunately, no industry-wide standard currently exists to quantify the characteristics of the signal. However, signal amplitude metrics among the different vendors provide quantities that can be found to have a linear relationship. One notable characteristic is the amplitude of the signal modulation. Other methods to characterize the quality of the pulsatile wave may be employed. It is not required for a pulse oximeter to support this feature.

5.5 Derived data

5.5.1 Limit indications

Pulse oximeters may implement indicators based on monitoring physiological values as falling outside predefined limits. The commonly implemented indicators include reaching the thresholds of a high or low SpO₂, or reaching the thresholds of a high or low pulse rate.

5.5.2 Pulsatile status

Pulse oximeters may provide status indications of certain characteristics of a pulsatile wave or irregularities in the waveform.

5.5.3 Device and sensor status

Pulse oximeters may provide status indications pertaining to sensor malfunction or dislodgement as well as various signal anomalies.

5.6 Stored data

As stated in 5.3.2.4, a pulse oximeter may be used over one or more sessions of several hours without being in contact with a manager to send its data. After the session or sessions are completed, the pulse oximeter agent connects to a manager. The manager is able to select which of the agent's stored sessions to retrieve. The agent then transmits the manager's selection in one or several blocks of messages for processing by a manager or other processing apparatus. The manager is also able to choose a set of sessions for deletion.

5.7 Device configurations

Although agents typically have a static configuration, it is permissible and desirable for an agent to support multiple configurations, one of which would be active at any given time. Pulse oximeters may have a rich set of features that can be combined into a collection of different configurations, one of which can be selected by the manager during configuration.

Two general categories of configurations exist. The first category is known as the set of standard configurations. These are intended to describe a relatively limited feature set of a single device specialization, which have predefined configuration identity (ID) codes. Managers may be pre-loaded with these configurations, in which case the configuration process is eliminated and immediate operation is allowed. The second category involves the set of extended configurations. These configurations are more flexible in that they may include concepts particular to one or more device specializations or include other features as defined in this standard.

6. Pulse oximeter DIM

6.1 Overview

This clause describes the DIM of the pulse oximeter.

6.2 Class extensions

In this standard, no class extensions are defined with respect to IEEE Std 11073-20601-2019.

6.3 Object instance diagram

The object instance diagram of the pulse oximeter DIM's numeric objects, defined for the purposes of this standard, is shown in Figure 1.

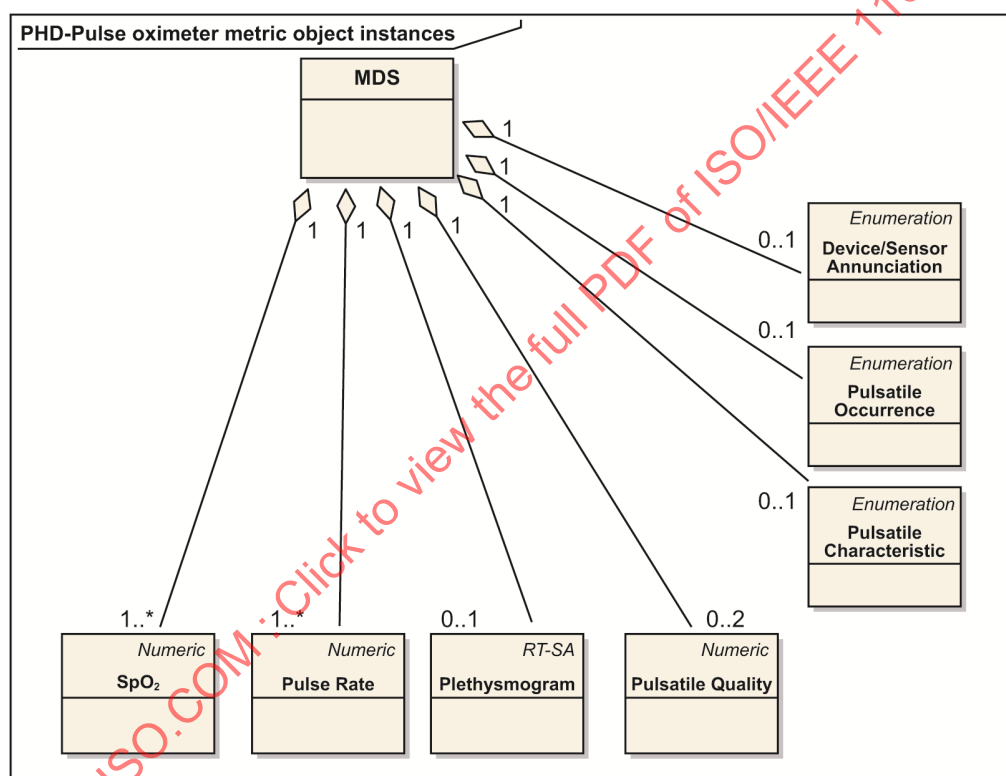


Figure 1—Pulse oximeter DIM for metric objects

The objects of the DIM, as shown in Figure 1, are described in the following subclauses: medical device system (MDS) object (see 6.5), the numeric objects (see 6.6), the real-time sample array (RT-SA) objects (see 6.7), and the enumeration objects (see 6.8). Figure 2 illustrates the PM-store objects (see 6.9), and the scanner objects (see 6.10) are shown in Figure 4. See 6.11 for rules for extending the pulse oximeter information model beyond elements as described in this standard. Each subclause that describes an object of the pulse oximeter contains the following information:

- The nomenclature code used to identify the class of the object. One example where this code is used is the configuration event, where the object class is reported for each object. This allows the manager to determine whether the class of the object being specified is a numeric, RT-SA, enumeration, scanner, or PM-store class.

- The attributes of the object. Each object has attributes that represent and convey information on the physical device and its data sources. Each object has a Handle attribute that identifies the object instance within an agent. Attribute values are accessed and modified using methods such as GET and SET. Attribute types are defined using ASN.1. The ASN.1 definitions for new attribute types specific to this standard are in Annex B, and the ASN.1 definitions for existing attribute types referenced in this standard are in IEEE Std 11073-20601-2019.
- The methods available on the object.
- The potential events generated by the object. Data are sent to the manager using events.
- The available services such as getting or setting attributes.

The attributes for each class are defined in tables that specify the name of the attribute, its value, and its qualifier. The qualifiers are as follows:

- M – Attribute is Mandatory, C – Attribute is Conditional and depends on the condition stated in the Remark or Value column (if IEEE Std 11073-20601-2019 is referenced, then it contains the conditions), R – Attribute is Recommended, O – Attribute is Optional, NR – Attribute is Not Recommended and NA – Attribute is Not Allowed. Mandatory attributes shall be implemented by an agent. Conditional attributes shall be implemented if the condition applies and may be implemented otherwise. Recommended attributes should be implemented by the agent. Optional attributes may be implemented on an agent. Not recommended attributes should not be implemented by the agent. If any attribute defined in the DIM of IEEE Std 11073-20601-2019 is not included in the definition of that object in this standard, it shall not be included in that object by an implementation. Vendor-specific attributes are allowed as described in 6.12.

An attribute is further qualified as static, dynamic, or observational. Static attributes shall not change value during the life of an association. Dynamic attributes have a value that may change during the life of an association. The dynamic attribute value should be sent at configuration time and shall be sent at or before the time when the value would be needed for interpreting a reported observation. Observational attributes have a value that may change during the life of an association. When a set of observational attribute values are received, these values are combined with the available context information (i.e., all related dynamic and static attribute values) to represent the observation at the observation time.

6.4 Types of configuration

6.4.1 General

As specified in IEEE Std 11073-20601-2019, two styles of configuration are available. The following subclauses briefly introduce standard and extended configurations.

6.4.2 Standard configuration

Standard configurations are defined in the ISO/IEEE 11073-104zz specializations (such as this standard) and are assigned a well-known identifier (Dev-Configuration-Id). The usage of a standard configuration is negotiated at configuration time between the agent and manager. If the manager acknowledges that it recognizes and wants to operate using the configuration, then the agent can begin sending measurements immediately. If the manager does not understand the configuration, the agent provides the configuration prior to transmitting measurement information.

6.4.3 Extended configuration

In extended configurations, the agent's configuration is not predefined in a standard. The agent determines which objects, attributes, and values that it wants to use in a configuration and assigns a configuration identifier. When the agent associates with a manager, it negotiates an acceptable configuration. Typically,

the manager does not know the agent's configuration on the first connection. Therefore, the manager responds that it needs the configuration and the agent transmits its configuration information by sending a configuration event report. If the manager already recognizes the configuration, either because it was preloaded via an installation program or the agent previously associated with the manager, then the manager responds that the configuration is known and no further configuration information needs to be sent.

If the device uses concepts and terms outside of this device specialization or terms defined in the private partition of IEEE 11073-10101, it is considered a proprietary device.

6.5 MDS object

6.5.1 MDS object attributes

Table 1 summarizes the attributes of the pulse oximeter MDS object. The nomenclature code to identify the MDS class is MDC_MOC_VMS_MDS_SIMP.

If a standard configuration is chosen, the timestamp type of MDS shall be consistent with the timestamp type of the metric objects in the chosen standard configuration.

In the response to a Get MDS Object command, only implemented attributes and their corresponding values are returned.

See IEEE Std 11073-20601-2019 for descriptive explanations of the individual attributes as well as information on attribute ID and attribute type.

The Dev-Configuration-Id attribute holds a locally unique 16-bit identifier that identifies the device configuration. For a pulse oximetry agent with extended configuration, this identifier is chosen in the range of extended-config-start to extended-config-end (see IEEE Std 11073-20601-2019) as shown in Table 1. The agent sends the Dev-Configuration-Id during the Associating state (see 8.3) to identify its configuration for the duration of the association. If the manager already holds the configuration information relating to the Dev-Configuration-Id, it recognizes the Dev-Configuration-Id. Then the Configuring state (see 8.4) is skipped, and the agent and manager enter the Operating state. If the manager does not recognize the Dev-Configuration-Id, the agent and manager enter the Configuring state.

If an agent implements multiple IEEE 11073-104zz specializations, System-Type-Spec-List is a list of type/version pairs, each referencing the respective device specialization and version of that specialization.

Table 1—MDS object attributes

Attribute name	Value	Qual.		
		Extended configuration	Standard configuration (Dev-Configuration-Id = 0x0190 or 0x0191)	Standard configuration (Dev-Configuration-Id = 0x0192)
Handle	0	M	M	M
System-Type	Attribute not present. See IEEE Std 11073-20601-2019.	C	C	C
System-Model	{“Manufacturer”, “Model”}	M	M	M
System-Id	EUI-64	M	M	M
Dev-Configuration-Id	Standard config: 0x0190 (400) Standard config: 0x0191 (401) Standard config: 0x0192 (402) Extended configs: 0x4000–0x7FFF	M	M	M
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	C	C	C
Production-Specification	See IEEE Std 11073-20601-2019.	O	O	O
Mds-Time-Info	See IEEE Std 11073-20601-2019.	C	C	M
Date-and-Time	See IEEE Std 11073-20601-2019.	C	NR (0x0190) M (0x0191)	NA
Base-Offset-Time	See IEEE Std 11073-20601-2019.	R	NA	M
Relative-Time	See IEEE Std 11073-20601-2019.	C	C (0x0190) NR (0x0191)	NR
HiRes-Relative-Time	See IEEE Std 11073-20601-2019.	C	C (0x0190) NR (0x0191)	NR
Date-and-Time-Adjustment	See IEEE Std 11073-20601-2019.	C	C	C
Power-Status	onBattery or onMains	R	R	R
Battery-Level	See IEEE Std 11073-20601-2019.	R	R	R
Remaining-Battery-Time	See IEEE Std 11073-20601-2019.	R	R	R
Reg-Cert-Data-List	See IEEE Std 11073-20601-2019.	O	O	O
System-Type-Spec-List	{MDC_DEV_SPEC_PROFILE_PULS_OXIM, 2}	M	M	M
Confirm-Timeout	See IEEE Std 11073-20601-2019.	O	O	O

NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static or dynamic.

NOTE 2—See 6.3 for a description of the qualifiers.

6.5.2 MDS object methods

Table 2 defines the methods (actions) of the MDS object. These methods are invoked using the ACTION service. In Table 2, the Subservice type name column defines the name of the method. The Mode column defines whether the method is invoked as an unconfirmed action (i.e., roiv-cmip-action from IEEE Std 11073-20601-2019) or a confirmed action (i.e., roiv-cmip-confirmed-action). The Subservice type (action-type) column defines the nomenclature code to use in the action-type field of an action request and response (see IEEE Std 11073-20601-2019). The Parameters (action-info-args) column defines the associated ASN.1 data structure (see IEEE Std 11073-20601-2019 for ASN.1 definitions) to use in the action message for the action-info-args field of the request. The Results (action-info-args) column defines the structure to use in the action-info-args of the response.

Table 2—MDS object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—
	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTimeInvoke	—

— **Set-Time:**

This method allows the manager to set a real-time clock in the agent with the absolute time. The agent indicates whether the Set-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601-2019).

The Set-Time method can be supported only if the Absolute-Time-Stamp attribute is supported.

— **Set-Base-Offset-Time:**

This method allows the manager to set a real-time clock in the agent with the base time and offset. The agent indicates whether the Set-Base-Offset-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601-2019).

The Set-Base-Offset-Time method can be supported only if the Base-Offset-Time-Stamp attribute is supported.

Agents following only this device specialization and no others send event reports by using agent-initiated measurement data transmission. However, the manager may control transmission of data through use of the scanner object to send data.

6.5.3 MDS object events

Table 3 defines the events that can be sent by the pulse oximeter MDS object.

Table 3—Pulse oximeter MDS object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event-info)	Results (event-reply-info)
EVENT REPORT	MDS-Configuration-Event	Confirmed or Unconfirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp
	MDS-Dynamic-Data-Update-Var	Confirmed or Unconfirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReportInfoVar	—
	MDS-Dynamic-Data-Update-Fixed	Confirmed or Unconfirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReportInfoFixed	—
	MDS-Dynamic-Data-Update-MP-Var	Confirmed or Unconfirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar	—
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed or Unconfirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—

— **MDS-Configuration-Event:**

This event is sent by the pulse oximetry agent during the configuring procedure if the manager does not already know the pulse oximeter agent's configuration from past associations or because the manager has not been implemented to recognize the configuration according to the pulse oximeter device specialization. The event provides static information about the supported measurement capabilities of the pulse oximetry agent.

— **MDS-Dynamic-Data-Update-Var:**

This event provides dynamic measurement data from the pulse oximetry agent for the numeric and enumeration object(s). This is reported using a generic attribute list variable format. The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

— **MDS-Dynamic-Data-Update-Fixed:**

This event provides dynamic measurement data from the pulse oximeter agent for the numeric and enumeration objects. This is reported in the fixed format defined by the Attribute-Value-Map attribute of the object(s). The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

— **MDS-Dynamic-Data-Update-MP-Var:**

This is the same as MDS-Dynamic-Data-Update-Var, but allows inclusion of data from multiple people.

MDS-Dynamic-Data-Update-MP-Fixed:

This is the same as MDS-Dynamic-Data-Update-Fixed, but allows inclusion of data from multiple people.

NOTE—IEEE Std 11073-20601-2019 requires that managers support all of the MDS object events listed above.

6.5.4 Other MDS services

6.5.4.1 GET service

A pulse oximetry agent shall support the GET service, which is provided by the MDS object to retrieve the values of all implemented MDS object attributes. The GET service can only be invoked after the Manager has confirmed selection of the Agent's configuration.

The manager may request the MDS object attributes of the pulse oximeter agent, in which case the manager shall send the “Remote Operation Invoke | Get” message (see roiv-cmip-get in IEEE Std 11073-20601-2019) with the reserved MDS handle value of 0. The pulse oximeter agent shall report either a list or its entire set of attributes of its MDS object attributes to the manager using the “Remote Operation Response | Get” message (see rors-cmip-get in IEEE Std 11073-20601-2019). See Table 4 for a summary of the GET service including some message fields.

Table 4—Pulse oximeter MDS object GET service

Service	Subservice type name	Mode	Subservice type	Parameters	Result
GET	<na>	<implied confirmed>	<na>	GetArgumentSimple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list

See 8.5.2 for details on the procedure for getting the MDS object attributes.

6.5.4.2 SET service

The pulse oximeter specialization does not require an implementation to support the MDS object SET service. However, a pulse oximetry agent vendor may implement a private SET service for the limited purposes of setting private attributes, which avoids any notion of remote control of the pulse oximetry agent. The implementation conformance statement (ICS) table should include information related to accessing private attributes in this manner.

6.6 Numeric objects

6.6.1 General

The pulse oximeter DIM for metric objects (see Figure 1) contains one mandatory numeric object for expressing SpO₂, one mandatory numeric object for pulse rate, several optional numeric objects for additional SpO₂, pulse rate modalities, pulse amplitude, and the reporting of current settings of physiological threshold limits. These are described in 6.6.2, 6.6.3, and 6.6.4.

Sometimes, the interpretation of one attribute value in an object depends on other attribute values in the same object. For example, Unit-Code and Unit-LabelString provide context for the observed values. Whenever a contextual attribute changes, the agent shall report these changes to the manager using an MDS object event (see 6.5.3) prior to reporting any of the dependent values.

6.6.2 SpO₂

Table 5 summarizes the attributes for reporting an SpO₂ measurement. The nomenclature code to identify the numeric class is MDC_MOC_VMO_METRIC_NU. At least one SpO₂ numeric object shall be supported by a pulse oximeter agent.

Table 5—SpO₂ numeric object attributes

Attribute name	Extended configuration		Standard Configuration (Dev-Configuration-Id = 0x0190 or 0x0191)		Standard Configuration (Dev-Configuration-Id = 0x0192)	
	Value	Qual.	Value	Qual.	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M	1	M	1	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_SAT_O2}	M	{MDC_PART_SCADA, MDC_PULS_OXIM_SAT_O2}	M	{MDC_PART_SCADA, MDC_PULS_OXIM_SAT_O2}	M
Supplemental-Types	See NOTE 1 and NOTE 2.	C	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	NR	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	NR
Metric-Spec-Small	mss-avail-stored-data, mss-acc-agent-initiated. See NOTE 1 and NOTE 2.	M	mss-avail-stored-data, mss-acc-agent-initiated. See NOTE 1 and NOTE 2.	M	mss-avail-stored-data, mss-acc-agent-initiated. See NOTE 1 and NOTE 2.	M
Metric-Structure-Small	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Measurement-Status	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Unit-Code	MDC_DIM_PERCENT	M	MDC_DIM_PERCENT	M	MDC_DIM_PERCENT	M
Attribute-Value-Map	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	C	When Dev-Configuration-Id = 0x0190: MDC_ATTR_NU_VAL_OBS_BASIC When Dev-Configuration-Id = 0x0191: MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS	M	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_BO	M
Source-Handle-Reference	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Label-String	See IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Unit-LabelString	See IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	C	When Dev-Configuration-Id = 0x0190: Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	0x0190: NR	Attribute not allowed.	NA
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R	When Dev-Configuration-Id = 0x0191: See IEEE Std 11073-20601-2019. Attribute not allowed.	0x0191: M NA	See IEEE Std 11073-20601-2019.	M

Table 5—SpO₂ numeric object attributes (*continued*)

Attribute name	Extended configuration		Standard Configuration (Dev-Configuration-Id = 0x0190 or 0x0191)		Standard Configuration (Dev-Configuration-Id = 0x0192)	
	Value	Qual.	Value	Qual.	Value	Qual.
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Measure-Active-Period	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Compound-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Accuracy	See IEEE Std 11073-20601-2019.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	R
Alert-Op-State	If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	O	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	C	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	C
Current-Limits	If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	O	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	C	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	C
Alert-Op-Text-String	See IEEE Std 11073-20601-2019.	O	See IEEE Std 11073-20601-2019.	NR	See IEEE Std 11073-20601-2019.	NR

NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.

NOTE 2—See 6.3 for a description of the qualifiers.

6.6.2.1 SpO₂—Extended configuration

A pulse oximeter agent may instantiate more than one SpO₂ numeric object. Typically, a pulse oximeter contains a single SpO₂ numeric object. However, a pulse oximeter may contain multiple SpO₂ numeric objects if it is designed to transmit multiple modalities of SpO₂ either successively or concurrently.

For a pulse oximeter agent with extended configuration, the AttrValMap structure (see IEEE Std 11073-20601) of the Attribute-Value-Map attribute may need to accommodate information pertaining to threshold status information in addition to other attributes such as the observed value and timestamp information.

The Supplemental-Types attribute is used to distinguish the modality of a particular SpO₂ measurement. In order to express the fast-response SpO₂ measurement, MDC_MODALITY_FAST shall be used as the value for the Supplemental-Types attribute. In order to express the slow-response SpO₂ measurement, MDC_MODALITY_SLOW shall be used as the value for the Supplemental-Types attribute. In order to express the spot-check SpO₂ measurement, MDC_MODALITY_SPOT shall be used as the value for the Supplemental-Types attribute. If there is no desire to distinguish a modality, the Supplemental-Types attribute shall not be used.

Certain combinations of Supplemental-Types are allowed. If it is desired to express that a spot-check measurement also uses a fast-response technique, the SupplementalTypeList structure of the Supplemental-Types attribute should contain the two values MDC_MODALITY_SPOT and MDC_MODALITY_FAST. Similarly, a spot-check using a slow-response measurement should contain the values MDC_MODALITY_SPOT and MDC_MODALITY_SLOW in its SupplementalTypeList. It is not recommended to combine the values MDC_MODALITY_SLOW and MDC_MODALITY_FAST.

The Metric-Spec-Small attribute may comprise several values, and one or more of these bits may be set:

- **mss-avail-stored-data:**
If this bit is set, the pulse oximeter agent may send up to 25 temporarily stored measurements in an event report.
- **mss-msmt-aperiodic:**
This bit is set if the measurement is not sent at a fixed interval. If a spot-check modality is used, this bit shall be set in addition to the use of the appropriate setting of the Supplemental-Types attribute. This bit may also be set when the spot-check modality is not used.
- **mss-acc-agent-initiated:**
This bit is set if the object's reportable values are transmitted via event reports. This does not mean that an agent shall send data in this manner, only that it is capable of doing so. This bit shall be set if this object reports its measurement data with an agent-initiated event report issued by the MDS object at any time during the association. If this object is scanned only by a scanner object (see 6.10), this bit shall not be set as the manager controls the data flow through the use of the Operational-State attribute. An agent implementation should make careful use of agent-initiated transfers that are not scanner objects, as the manager has little, if any, control of the bandwidth utilization of the data link. If agent-initiated transfers are used, they should be for either intermittent or periodic event reports of a small number of object values.

Exactly one among the Absolute-Time-Stamp and Base-Offset-Time-Stamp attribute in the SpO₂ numeric object shall be present when using the spot-check modality.

6.6.2.1.1 Threshold settings and status attributes

Three attributes (Alert-Op-State, Current-Limits, Alert-Op-Text-String) of the SpO₂ numeric object are provided to report the threshold settings of agent, and the Measurement-Status attribute reports the threshold status, i.e., whether the measurement has reached or crossed beyond the threshold boundaries.

The Current-Limits attribute stores the threshold values as FLOAT-Type values. If a Basic-Nu-Observed-Value attribute is used to express the measurement value, the values in the Current-Limits attribute shall be expressed within the range and precision of a SFLOAT value.

6.6.2.2 SpO₂—Standard configurations

The first standard configuration defined in this standard contains two numeric objects, one of which is the SpO₂ numeric object, described in the Standard Configuration column in Table 1. This standard configuration is provided to describe a most basic pulse oximeter implementation.

A second standard configuration is intended for spot-check use cases. In addition to assigning the Dev-Configuration-Id to 0x0191, the SpO₂ object attributes are modified from Dev-Configuration-Id = 0x0190 as follows:

- The Supplemental-Types attribute shall contain a single entry in its SupplementalTypeList, and its value shall be MDC_MODALITY_SPOT.
- The AttrValMap structure (see IEEE Std 11073-20601) of the Attribute-Value-Map attribute differs from Table 5 in that it shall contain the attribute ID and attribute length information of the Basic-Nu-Observed-Value and Absolute-Time-Stamp (or Base-Offset-Time-Stamp) attribute in this stated order.
- The Metric-Spec-Small attribute shall set the following two bits appropriately:
- **mss-avail-stored-data:**
If this bit is set, the pulse oximeter agent may send up to 25 temporarily stored measurements in an event report.
- **mss-acc-agent-initiated:**
Since the standard configuration contains two numeric objects, the bandwidth requirements are intended to be relatively light.

If an implementation is more capable than that provided by either of these standard configurations, it shall use an extended configuration.

The third standard configuration has the Dev-Configuration-Id=0x0192. It is the ‘Base-Offset-Time’ version of the second standard configuration (Dev-Configuration-Id=0x0191). The only difference between them is the format of timestamp, and correspondingly the content of Attribute-Value-Map.

6.6.2.3 SpO₂—Methods, events, services

The SpO₂ numeric object does not support any methods, events, or other services.

See IEEE Std 11073-20601-2019 for descriptive explanations of the individual attributes as well as information on attribute ID and attribute type.

6.6.3 Pulse rate

Table 6 summarizes the attributes for reporting a pulse rate measurement. The nomenclature code to identify the numeric class is MDC_MOC_VMO_METRIC_NU. At least one pulse rate numeric object shall be supported by a pulse oximeter agent.

Table 6—Pulse rate numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x0190 or 0x0191)		Standard configuration (Dev-Configuration-Id = 0x0192)	
	Value	Qual.	Value	Qual.	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M	10	M	10	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_PULS_RATE}	M	{MDC_PART_SCADA, MDC_PULS_OXIM_PULS_RATE}	M	{MDC_PART_SCADA, MDC_PULS_OXIM_PULS_RATE}	M
Supplemental- Types	See NOTE 1 and NOTE 2.	C	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	NR	See IEEE Std 11073-20601-2019 and NOTE 1 and NOTE 2.	NR
Metric-Spec- Small	mss-avail-stored-data, mss-acc- agent-initiated. See NOTE 1 and NOTE 2.	M	mss-avail-stored-data, mss-acc- agent-initiated. See NOTE 1 and NOTE 2.	M	mss-avail-stored-data, mss-acc- agent-initiated. See NOTE 1 and NOTE 2.	M
Metric- Structure-Small	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Measurement- Status	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Metric-Id- Partition	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Unit-Code	MDC_DIM_BEAT_PER_MIN	M	MDC_DIM_BEAT_PER_MIN	M	MDC_DIM_BEAT_PER_MIN	M
Attribute- Value-Map	See IEEE Std 11073-20601-2019.	C	When Dev-Configuration-Id = 0x0190: MDC_ATTR_NU_VAL_OBS_BASIC When Dev-Configuration-Id = 0x0191: MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS	M	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_BO	M
Source-Handle- Reference	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Label-String	See IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Unit- Label-String	See IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	O
Absolute-Time- Stamp	See IEEE Std 11073-20601-2019.	C	When Dev-Configuration-Id = 0x0190: Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	0x0190: NR	Attribute not allowed.	NA
Base-Offset- Time-Stamp	See IEEE Std 11073-20601-2019.	R	When Dev-Configuration-Id = 0x0191: See IEEE Std 11073-20601-2019.	0x0191: M		
			Attribute not allowed.	NA	See IEEE Std 11073-20601-2019.	M

Table 6—Pulse rate numeric object attributes (*continued*)

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x0190 or 0x0191)		Standard configuration (Dev-Configuration-Id = 0x0192)	
	Value	Qual.	Value	Qual.	Value	Qual.
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Measure-Active-Period	See IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	NR
Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C	See IEEE Std 11073-20601-2019. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2019 apply.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Compound-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	C
Accuracy	See IEEE Std 11073-20601-2019.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601-2019.	R
Alert-Op-State	If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	O	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	NR	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	NR
Current-Limits	If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	O	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	NR	Attribute initially not present. If thresholding is to be used, this attribute is mandatory. See IEEE Std 11073-20601-2019.	NR
Alert-Op-Text-String	See IEEE Std 11073-20601-2019.	O	See IEEE Std 11073-20601-2019.	NR	See IEEE Std 11073-20601-2019.	NR

NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.

NOTE 2—See 6.3 for a description of the qualifiers.

6.6.3.1 Pulse rate—Extended configuration

A pulse oximeter agent may instantiate more than one pulse rate numeric object. Typically, a pulse oximeter contains a single pulse rate numeric object. However, a pulse oximeter may contain multiple pulse rate numeric objects if it is designed to transmit multiple modalities of pulse rate either successively or concurrently.

For a pulse oximeter agent with extended configuration, the AttrValMap structure (see IEEE Std 11073-20601-2019) of the Attribute-Value-Map attribute may need to accommodate information pertaining to threshold status information in addition to other attributes such as the observed value and timestamp information.

The Supplemental-Types attribute is used to distinguish the modality of a particular pulse rate measurement. In order to express a fast-response pulse rate measurement, MDC_MODALITY_FAST shall be used in the Supplemental-Types attribute. In order to express a slow-response pulse rate measurement, MDC_MODALITY_SLOW shall be used in the Supplemental-Types attribute. In order to express the single spot-check pulse rate measurement, MDC_MODALITY_SPOT shall be used in the Supplemental-Types attribute. If there is no desire to distinguish a modality, the Supplemental-Types attribute shall not be used.

Certain combinations of Supplemental-Types are allowed. If it is desired to illustrate that a spot-check measurement also uses a fast-response technique, the SupplementalTypeList structure of the Supplemental-Types attribute should contain the two values MDC_MODALITY_SPOT and MDC_MODALITY_FAST. Similarly, a spot-check using a slow-response measurement should contain the values MDC_MODALITY_SPOT and MDC_MODALITY_SLOW in its SupplementalTypeList. It is not recommended to combine the values MDC_MODALITY_SLOW and MDC_MODALITY_FAST.

The Metric-Spec-Small attribute may comprise several values, and one or more of these bits may be set:

- **mss-avail-stored-data:**
If this bit is set, the pulse oximeter agent may send up to 25 temporarily stored measurements in an event report.
- **mss-msmt-aperiodic:**
This bit is set if the measurement is not sent at a fixed interval. If a spot-check modality is used, this bit shall be set in addition to the use of the appropriate setting of the Supplemental-Types attribute. This bit may also be set when the spot-check modality is not used.
- **mss-acc-agent-initiated:**
This bit is set if the object's reportable values are transmitted via event reports. This does not mean that an agent shall send data in this manner, only that it is capable of doing so. This bit shall be set if this object reports its measurement data with an agent-initiated event report issued by the MDS object at any time during the association. If this object is scanned only by a scanner object (see 6.10), this bit shall not be set as the manager controls the data flow through the use of the Operational-State attribute. An agent implementation should make careful use of agent-initiated transfers that are not scanner objects, as the manager has little, if any, control of the bandwidth utilization of the data link. If agent-initiated transfers are used, they should be for either intermittent or periodic event reports of a small number of object values.

Exactly one among the Absolute-Time-Stamp and Base-Offset-Time-Stamp attribute in the pulse rate numeric object shall be present when using the spot-check modality.

6.6.3.1.1 Threshold settings and status attributes

See 6.6.2.1.1.

6.6.3.2 Pulse rate—Standard configuration

The first standard configuration defined in this standard contains two numeric objects, one of which is the pulse rate numeric object, described in the Standard Configuration column in Table 6. The standard configuration is provided to describe a most basic pulse oximeter implementation.

A second standard configuration is intended for spot-check use cases. In addition to assigning the Dev-Configuration-Id to 0x0191, the pulse rate object attributes are modified from Dev-Configuration-Id = 0x0190 as follows:

- The Supplemental-Types attribute shall contain a single entry in its SupplementalTypeList, and its value shall be MDC_MODALITY_SPOT.
- The AttrValMap structure (see IEEE Std 11073-20601) of the Attribute-Value-Map attribute differs from Table 6 in that it shall contain the attribute ID and attribute length information of the Basic-Nu-Observed-Value and Absolute-Time-Stamp (or Base-Offset-Time-Stamp) attribute in this stated order.
- The Metric-Spec-Small attribute shall set the following two bits appropriately:
- **mss-avail-stored-data:**
If this bit is set, the pulse oximeter agent may send up to 25 temporarily stored measurements in an event report.
- **mss-acc-agent-initiated:**
Since the standard configuration contains two numeric objects, the bandwidth requirements are intended to be relatively light.

If an implementation is more capable than that provided by this standard configuration, it shall use an extended configuration.

The third standard configuration has the Dev-Configuration-Id=0x0192. It is the ‘Base-Offset-Time’ version of the second standard configuration (Dev-Configuration-Id=0x0191). The only difference between them is the format of timestamp, and correspondingly the content of Attribute-Value-Map.

6.6.3.3 Pulse rate—Methods, events, services

The pulse rate numeric object does not support any methods, events, or other services.

See IEEE Std 11073-20601-2019 for descriptive explanations on the individual attributes as well as information on attribute ID and attribute type.

6.6.4 Pulsatile quality

Pulse oximeter vendors have various methods to express pulse amplitude, perfusion factor, or similar measure. These methods may comprise complex averaging formulas, scaling factors, and the like. In many cases, these various methods result in measurements that differ by a constant scaling value, but no standardized methodology currently exists to unify the notion of such a metric.

This numeric object serves as a container for expressing a quantifying element, which could be the modulation of the pulsatile signal or some other formulation, and agent implementers may choose the methods and attributes to express this numeric.

Since there are multiple ways to quantify the pulsatile waveform, more than one of these objects may be instantiated. For instance, one object can contain a pulse amplitude measurement, and a second object could contain some formulation of a defined pulsatile index.

Agent implementers should describe the implementation in the ICS tables described in Table 25 and Table 26. Information suitable for the DIM MOC ICS table should include the following:

- General implementation support of the measurement
- Commentary relating to guiding the use of the measurement value

Information suitable for the MOC attribute ICS table should include the following:

- Background on any unit code that may be used
- Description of any averaging method used
- Description of normalization values (e.g., the number reported is related to a root-mean-square value of peak)
- Information on which wavelength or wavelengths are used to calculate the measurement

Table 7 summarizes the attributes for building a framework to assist in expressing pulsatile quality.

Table 7—Pulsatile quality numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_PERF_REL} or {MDC_PART_SCADA_MDC_SAT_O2_QUAL}	M
Supplemental-Types	See IEEE Std 11073-20601-2019.	NR
Metric-Spec-Small	mss-acc-agent-initiated	M
Metric-Structure-Small	See IEEE Std 11073-20601-2019.	NR
Measurement-Status	See IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	O
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2019.	NR
Unit-Code	See NOTE 1 and NOTE 2.	O
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	O
Source-Handle-Reference	See IEEE Std 11073-20601-2019.	O
Label-String	See NOTE 1 and NOTE 2.	R
Unit-LabelString	See NOTE 1 and NOTE 2.	R
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Measure-Active-Period	See IEEE Std 11073-20601-2019.	O
Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Compound-Nu-Observed-Value	See IEEE Std 11073-20601-2019.	C
Accuracy	See IEEE Std 11073-20601-2019.	O
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

The unit code MDC_DIM_DIMLESS is the recommended dimension if this object is expressing a form of pulse amplitude, indicated by the type field set to MDC_PULS_OXIM_PERF_REL. Private unit codes may be used at the implementer's discretion, but could hinder the interoperability of the personal health infrastructure. If the type field contains MDC_SAT_O2_QUAL, the recommended dimension is MDC_DIM_PERCENT.

Similarly, the Label-String and Unit-LabelString attributes would be useful in conveying to the user more information regarding the characteristic being conveyed.

The pulsatile quality numeric object does not support any methods, events, or other services.

See IEEE Std 11073-20601-2019 for descriptive explanations on the individual attributes as well as information on attribute ID and attribute type.

6.7 Real-time sample array (RT-SA) objects

6.7.1 Plethysmographic waveform

A representation of the pulsatile wave may be transmitted as a series of samples.

Table 8 defines the attributes of the plesythmogram RT-SA object. This object is optional for this standard. The nomenclature code to identify the RT-SA object class is MDC_MOC_VMO_METRIC_SA_RT.

Table 8—Plethysmogram object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_PLETH }	M
Supplemental-Types	See IEEE Std 11073-20601-2019.	NR
Metric-Spec-Small	See NOTE 1 and NOTE 2.	M
Measurement-Status	See IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR
Unit-Code	See NOTE 1 and NOTE 2.	O
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	C
Source-Handle-Reference	See NOTE 1 and NOTE 2.	O
Label-String	See IEEE Std 11073-20601-2019.	O
Unit-LabelString	See IEEE Std 11073-20601-2019.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Sample-Period	See IEEE Std 11073-20601-2019.	M
Simple-Sa-Observed-Value	See IEEE Std 11073-20601-2019.	M
Scale-and-Range-Specification	See IEEE Std 11073-20601-2019.	M
Sa-Specification	See IEEE Std 11073-20601-2019.	M
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

An agent should use the unit code of MDC_DIM_DIMLESS units as the basic value, as the sample points are often expressed as dimensionless units.

Several attributes in the plethysmogram are optional, and such flexibility allows implementations reasonable latitude in expressing details that the various vendors deem significant.

The plethysmogram data should be made available only through a scanner object. Asserting the mss-acc-agent-initiated bit is not recommended, as this implies that this object's data are transmitted via MDS event reports.

NOTE—The values in the RT-SA are intended to represent a plethysmogram, and these values may be related to the same values used to convey pulse amplitude information. The common practice of displaying a plethysmogram is such that the profile of the waveform will be an inversion of the absorbance waveform, in that a pulsatile inrush is seen as an upward deflection on a display. The manager is not required to perform any post-processing in order to invert the waveform, but the manager may need to be aware of this difference in order to present a more viewable waveform.

6.8 Enumeration objects

6.8.1 General

The pulse oximeter DIM (see Figure 1) contains three optional enumeration objects. The Pulsatile Occurrence enumeration object informs the user when a pulsatile wave is detected. The Pulsatile Characteristic object provides additional information about the pulsatile occurrence. Finally, an enumeration object is provided to enable an agent to report additional conditions concerning sensor status, general signal conditions, and device status in the device and sensor annunciation status object.

6.8.2 Pulsatile occurrence

Pulse oximeters often convey that they are detecting a pulsatile occurrence. One application of this object is to facilitate the flashing of a real-time display icon each time a pulsatile event is reported. Another application involves the ability to precisely timestamp the maximal inrush of a pulsatile wave. The nomenclature code to identify the enumeration object class is MDC_MOC_VMO_METRIC_ENUM. Refer to Table 9 for the set of attributes of this object.

This object is instantiated only in extended configurations, and it is optional to instantiate, but enables the ability to report the occurrence of a pulse. A manager should support the interpretation of this object in order to indicate the occurrence of a pulse.

If the Source-Handle-Reference is defined, it should point to either the Pulsatile Quality numeric object or the Plethysmogram RT-SA object.

Explicit expression of the existence of a pulsatile event is realized by sending the appropriate value in the Enum-Observed-Value-Simple-OID attribute. When reporting that a pulsatile occurrence has occurred, the value sent shall be MDC_TRIG_BEAT. If reporting that the maximal inrush of the pulsatile wave has occurred, the value sent shall be MDC_TRIG_BEAT_MAX_INRUSH.

The precise definition of “maximal inrush” in terms of slope or amplitude is vendor-dependent and should be defined in the appropriate ICS section.

If this object is sent within a periodic configurable scanner object and its object elements are reported using fixed format value messages (see 6.10.2), a placeholder value of MDC_METRIC_NOS may be sent to indicate that no pulsatile event occurred within the period that the Buf-Scan-Report-* event was emitted.

Table 9—Pulsatile occurrence enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Type	{MDC_PART_SCADA, MDC_TRIG }	M
Supplemental-Types	See IEEE Std 11073-20601-2019.	O
Metric-Spec-Small	mss-acc-agent-initiated	M
Metric-Structure-Small	See IEEE Std 11073-20601-2019.	NR
Measurement-Status	See IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2019.	NR
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	C
Source-Handle-Reference	See NOTE 1 and NOTE 2.	O
Label-String	See IEEE Std 11073-20601-2019.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601-2019.	R
Enum-Observed-Value-Simple-Bit-Str	See NOTE 1 and NOTE 2.	NR
Enum-Observed-Value-Basic-Bit-Str	See following text.	NR
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value	See NOTE 1 and NOTE 2.	NR
Enum-Observed-Value-Partition	See IEEE Std 11073-20601-2019.	O
Capability-Mask-Simple	See IEEE Std 11073-20601-2019.	NR
Capability-Mask-Basic	See IEEE Std 11073-20601-2019.	NR
State-Flag-Simple	See IEEE Std 11073-20601-2019.	NR
State-Flag-Basic	See IEEE Std 11073-20601-2019.	NR
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

6.8.3 Pulsatile characteristic

Pulse oximeters may convey additional information about the pulsatile wave. The Pulsatile Characteristic object includes indication of adequate perfusion. The nomenclature code to identify the enumeration object class is MDC_MOC_VMO_METRIC_ENUM. Refer to Table 10 for the set of attributes of this object.

This object is instantiated only in extended configurations, and it is optional to instantiate, but enables the ability to report certain pulsatile conditions or artifacts. A manager should support the interpretation of this object in order to indicate characteristic information about a pulsatile wave.

If the Source-Handle-Reference is defined, it should point to either the Pulse Amplitude numeric object or the Plethysmogram RT-SA object.

Table 10—Pulse characteristic enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_PULS_CHAR }	M
Supplemental-Types	See IEEE Std 11073-20601-2019.	O
Metric-Spec-Small	mss-acc-agent-initiated	M
Metric-Structure-Small	See IEEE Std 11073-20601-2019.	NR
Measurement-Status	See IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2019.	NR
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	C
Source-Handle-Reference	See NOTE 1 and NOTE 2.	O
Label-String	See IEEE Std 11073-20601-2019.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Simple-OID	One of the codes defined in Table 11.	R
Enum-Observed-Value-Simple-Bit-Str	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Basic-Bit-Str	See IEEE Std 11073-20601-2019.	O
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value	See NOTE 1 and NOTE 2.	NR
Enum-Observed-Value-Partition	See IEEE Std 11073-20601-2019.	O
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

Explicit expression of the existence of characteristic events is realized by sending OID code via the Enum-Observed-Value-Simple-OID attribute, as defined in Table 11. The Enum-Observed-Value attribute should not be used as it complicates the modeling of the object.

If a manager supports the interpretation of this object, it shall be able to interpret the entire set of presented characteristics, defined in Table 11. An agent is not required to implement all the features specified in Table 11. An agent shall report each time there is a change in status in a condition. Note that a manager shall interpret these OID codes only within the context of this attribute and only within this device specialization, as other specializations may use corresponding terms for different purposes.

Table 11—Mapping of pulse characteristics to object OID attribute

Pulsatile characteristic	Codes
Quality of the detected pulse is nominal, in that there are no recognized abnormalities in the detected pulse.	MDC_PULS_OXIM_PULS_CHAR_NOMINAL
Perfusion or quality of the detected pulse is marginal.	MDC_PULS_OXIM_PULS_CHAR_MARGINAL
Perfusion or quality of the detected pulse is minimal.	MDC_PULS_OXIM_PULS_CHAR_MINIMAL
Perfusion or quality of the detected pulse is unacceptable.	MDC_PULS_OXIM_PULS_CHAR_UNACCEPTABLE

6.8.4 Device and sensor annunciation conditions

The device and sensor annunciation status object reports on several aspects of the pulse oximeter equipment, including sensor displacement, faulty sensor detection, signal irregularities and loss-of-signal-tracking, and low-perfusion determination. The status of each aspect is reported by a specific status bit.

The device and sensor annunciation object containing the running status of the device, general signal condition, and sensor assembly is also provided. If this object is to be implemented, then the OID-Type and bit assignments shall be implemented as described in this subclause. Status bits in this object are distinguished from similar bits in the Pulsatile Characteristic object in that information in this object pertain to the general signal condition, whereas those in the Pulsatile Characteristic object are limited to a single pulsatile occurrence. The nomenclature code to identify the enumeration object class is MDC_MOC_VMO_METRIC_ENUM. Refer to Table 12 for the set of attributes of this object.

Table 12—Device and sensor annunciation status object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Type	{MDC_PART_SCADA, MDC_PULS_OXIM_DEV_STATUS }.	M
Supplemental-Types	See IEEE Std 11073-20601-2019.	O
Metric-Spec-Small	mss-acc-agent-initiated.	M
Metric-Structure-Small	See IEEE Std 11073-20601-2019.	NR
Measurement-Status	See IEEE Std 11073-20601-2019.	O
Metric-Id	See IEEE Std 11073-20601-2019.	NR
Metric-Id-List	See IEEE Std 11073-20601-2019.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2019.	NR
Attribute-Value-Map	See IEEE Std 11073-20601-2019.	C
Source-Handle-Reference	See NOTE 1 and NOTE 2.	NR
Label-String	See IEEE Std 11073-20601-2019.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2019.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2019.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Simple-Bit-Str	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value-Basic-Bit-Str	See NOTE 1 and NOTE 2.	R
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601-2019.	NR
Enum-Observed-Value	See NOTE 1 and NOTE 2.	NR
Enum-Observed-Value-Partition	See IEEE Std 11073-20601-2019.	O
Capability-Mask-Simple	See IEEE Std 11073-20601-2019.	C
Capability-Mask-Basic	See IEEE Std 11073-20601-2019.	R
State-Flag-Simple	See IEEE Std 11073-20601-2019.	C
State-Flag-Basic	See IEEE Std 11073-20601-2019.	R
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static, observational, or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

This object is instantiated only in extended configurations. A manager should support the interpretation of this object to enable reporting of these conditions. An agent should support this object to transmit these conditions.

Similarly, the Source-Handle-Reference is inappropriate, as this object monitors the status of the equipment.

Explicit expression of the existence of annunciations is realized by the setting of the appropriate bit in the Enum-Observed-Value-Basic-Bit-Str attribute, as defined in Table 13. It is recommended to use the Enum-Observed-Value-Basic-Bit-Str attribute, as it consumes fewer payload octets than the Enum-Observed-Value-Simple-Bit-Str attribute. The Enum-Observed-Value attribute should not be used, as it unnecessarily complicates the modeling of the object. If a manager supports the interpretation of this object, it shall be able to interpret the entire set of presented conditions, defined in Table 13 by the PulseOxDevStat entity. An agent is not required to implement all the features specified in Table 13. An agent shall report each time there is a change in status in a condition. Note that a manager shall interpret these bits only within the context of this attribute and only within this device specialization as other specializations may use corresponding terms for different purposes.

Table 13—Mapping of device, sensor and signal status to object Bit-Str attribute

Device or sensor condition	PulseOxDevStat mnemonic
Agent reports that the sensor is disconnected from the instrument.	sensor-disconnected
Agent reports that the sensor is malfunctioning or faulting.	sensor-malfunction
Agent reports that the sensor is not properly attached or has been dislodged, and accurate measurement is, therefore, prevented.	sensor-displaced
An unsupported sensor is connected to the agent.	sensor-unsupported
Agent reports that sensor is not connected to the user.	sensor-off
Agent reports that there is interference due to ambient light or electrical phenomena.	sensor-interference
Signal analysis is currently in progress prior to measurement availability.	signal-searching
Agent determines that a questionable pulse is detected.	signal-pulse-questionable
Agent detects a nonpulsatile signal.	signal-non-pulsatile
Agent reports that the signal is erratic or is not plausible.	signal-erratic
Agent reports a consistently low perfusion condition exists.	signal-low-perfusion
Agent reports a poor signal exists, possibly affecting accuracy.	signal-poor
Agent reports that the incoming signal cannot be analyzed or is inadequate for producing a meaningful result.	signal-inadequate
Agent has determined that some irregularity has been detected while processing the signal.	signal-processing-irregularity
A general device fault has occurred in the agent.	device-equipment-malfunction
An extended display update is currently active.	device-extended-update

The specific bit mappings of PulseOxDevStat are defined in B.1.

6.9 PM-store objects

6.9.1 General

Several use cases illustrate that a pulse oximetry agent may store many minutes or hours worth of oximetry data while unable to remain in communication with a manager, or it is impractical to send multiple event reports of blocks of temporarily stored measurements. After the long-term acquisition is complete, the manager retrieves the data from the agent. This mechanism is allowed in extended configurations.

6.9.2 Persistent store model

The wide range of potential combinations of data layouts makes it impractical to provide a specification for a single normative persistent store data model. As such, a pulse oximetry agent has considerable latitude in selecting the format and set of data elements to transmit. If a pulse oximetry agent supports this function, the framework in the following subclause suggests a possible data layout. The intent of this approach is to provide a “file system description” of the data layout, as opposed to a “file format specification.” In other words, following the guides provided in this standard should enable an implementer to store and retrieve the data within this model, but the specifics for determining the specific nature of the data layout and the subsequent visualization, mining, or other managing of the retrieved data is outside the scope of this standard.

The pulse oximeter in this use case stores oximetry data in a number of different ways, depending on the particular needs of the acquisition. The information model for the persistent store hierarchy is shown in Figure 2. As an example and pattern, Figure 3 illustrates the relationship between the various objects for the PM-store implementation. The PM-segments could group data in different ways. It could contain all varieties of data within one session, or multiple PM-segments could be created, with one containing all SpO₂ measurements for the session and a second containing all pulse rate measurements for that same session. However, the hierarchy of the PM-segment, entry, and elements should take the form seen in Figure 3.

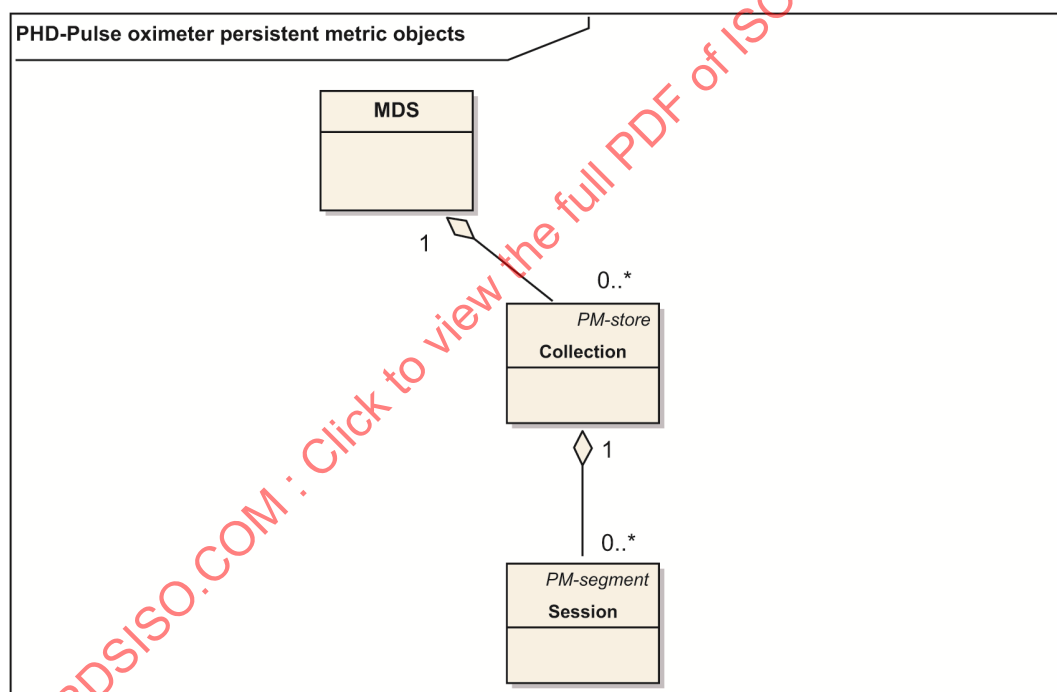


Figure 2—Pulse oximeter DIM for the PM-store hierarchy

This example illustrates a PM-store realization with two PM-segments. In this case, each PM-segment stores data from a distinct contiguous session. Figure 3 shows each PM-segment entry containing two data elements: the first representing an SpO₂ measurement and the second representing a pulse rate measurement. Since each entry contains the set of consistently ordered data sampled at a single point in time, one could place timestamp information in the SegEntryHdr, indicating the occurrence of each reading. If the samples are taken at fixed intervals, then the start time and sampling interval should be stored in the PM-segment attributes MDC_ATTR_TIME_START_SEG and MDC_ATTR_TIME_PD_SAMP, and the SegEntryHdr may be left empty, whereas if the samples are not taken at fixed intervals, the timestamp of each sample must be stored in each SegEntryHdr.

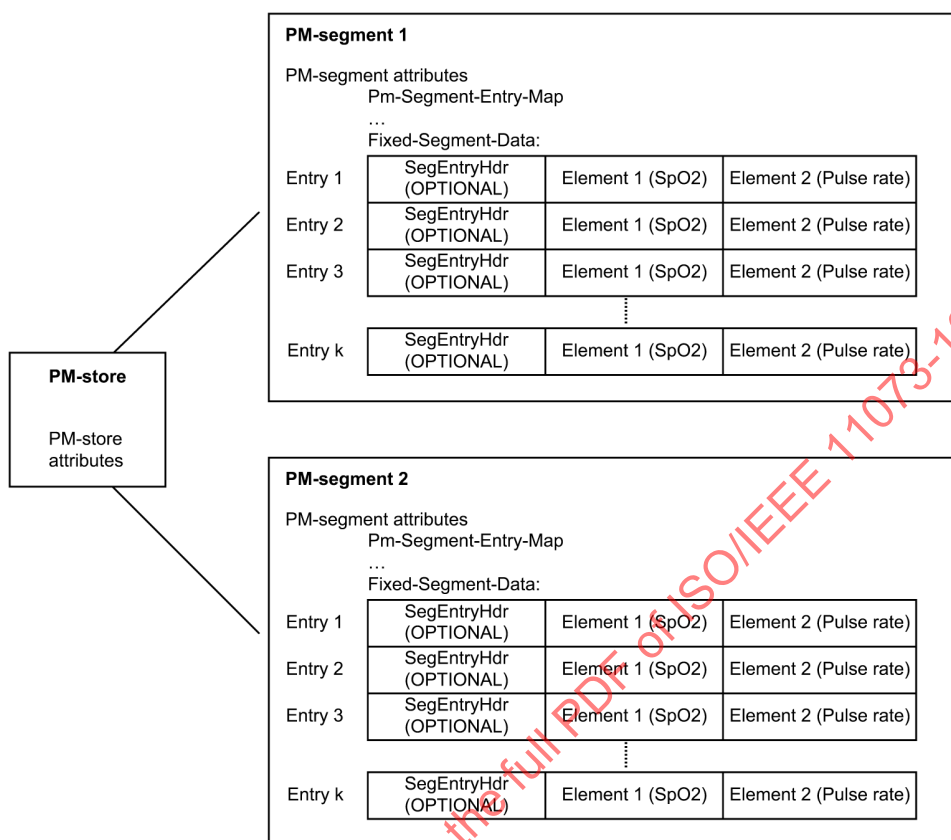


Figure 3—PM-store usage for pulse oximeter

6.9.3 PM-store object attributes

Table 14 lists the attributes for the PM-store object.

Table 14 —PM-store object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
PM-Store-Capab	See IEEE Std 11073-20601-2019.	M
Store-Sample-Algorithm	See IEEE Std 11073-20601-2019.	M
Store-Capacity-Count	See IEEE Std 11073-20601-2019.	O
Store-Usage-Count	See IEEE Std 11073-20601-2019.	O
Operational-State	See IEEE Std 11073-20601-2019.	M
PM-Store-Label	See IEEE Std 11073-20601-2019.	O
Sample-Period	See IEEE Std 11073-20601-2019.	C
Number-Of-Segments	See IEEE Std 11073-20601-2019.	M
Clear-Timeout	See IEEE Std 11073-20601-2019.	M
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

6.9.4 PM-store object methods

Table 15 defines the methods used by the PM-store object.

Table 15—PM-store object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	-
	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList
	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmDataXferReq	TrigSegmDataXferRsp

6.9.5 PM-store object events

Table 16 defines the events sent by the PM-store object.

Table 16—PM-store object events

Event	Mode	Event type	Event info parameter	Event-reply-info
Segment-Data-Event	Confirmed	MDC_NOTI_SEGMENT_DATA	SegmentDataEvent	SegmentDataResult

To facilitate a practical level of device support, a Segment-Data-Event report size shall be no larger than 8192 octets. A PM-segment containing data in excess of this size shall transfer its data using multiple Segment-Data-Event reports as described in IEEE Std 11073-20601-2019.

6.9.6 PM-store object services

The GET service shall be provided by an agent implementing one or more PM-store objects. This service shall be available while the agent is in the Operating state. Refer to IEEE Std 11073-20601-2019 for further details.

6.9.7 PM-segment objects

Table 17 defines the attributes of the PM-segment object contained in the PM-store object managing the stored measurements. The nomenclature code to identify the PM-segment class is MDC_MOC_PM_SEGMENT.

The Fixed-Segment-Data attribute serves as the container of the stored measurements. The exact data format or data type of this attribute is vendor-specific.

Table 17—PM-segment object attributes

Attribute name	Extended configuration	
	Value	Qual.
Instance Number	See IEEE Std 11073-20601-2019.	M
PM-Segment-Entry-Map	See IEEE Std 11073-20601-2019.	M
PM-Seg-Person-Id	See IEEE Std 11073-20601-2019.	C
Sample-Period	See IEEE Std 11073-20601-2019.	C
Operational-State	See IEEE Std 11073-20601-2019.	M
Segment-Label	See IEEE Std 11073-20601-2019.	O
Segment-Start-Abs-Time	See IEEE Std 11073-20601-2019.	NR
Segment-End-Abs-Time	See IEEE Std 11073-20601-2019.	NR
Date-and-Time-Adjustment	See IEEE Std 11073-20601-2019.	C
Segment-Start-BO-Time	See IEEE Std 11073-20601-2019.	R
Segment-End-BO-Time	See IEEE Std 11073-20601-2019.	R
Segment-Usage-Count	See IEEE Std 11073-20601-2019.	O
Segment-Statistics	See IEEE Std 11073-20601-2019.	O
Fixed-Segment-Data	Specified by vendor.	M
Confirm-Timeout	See IEEE Std 11073-20601-2019.	O
Transfer-Timeout	See IEEE Std 11073-20601-2019.	M

6.10 Scanner objects

6.10.1 General

The scanner object class is a powerful construct that enables efficient grouping of several metrics into a single payload. It is also helpful in conveying the continuous nature of annunciations expressed within enumeration objects, as the scanner object can periodically query or observe the enumeration object dedicated to a particular part of status recording. The information model for the scanner hierarchy is shown in Figure 4. The periodic or episodic configurable scanner objects are instantiated only in extended configurations. The nomenclature code to identify the periodic configurable scanner object class is MDC_MOC_SCAN_CFG_PERI, and the code to identify the episodic configurable scanner is MDC_MOC_SCAN_CFG_EPI.

A simple example of the scanner configuration and data reporting can be found in E.6.

The episodic configurable scanner can be used to send episodic observations, e.g., the pulse occurrence, only when these observations happen.

Since IEEE Std 11073-20601-2019 requires the manager to support grouped format event reports, a manager must support the interpretation of this object class if the agent transmits data using periodic or episodic scanner objects. Otherwise, if the agent presents the bulk of its data with scanner objects, the manager cannot receive the data presented by such an agent.

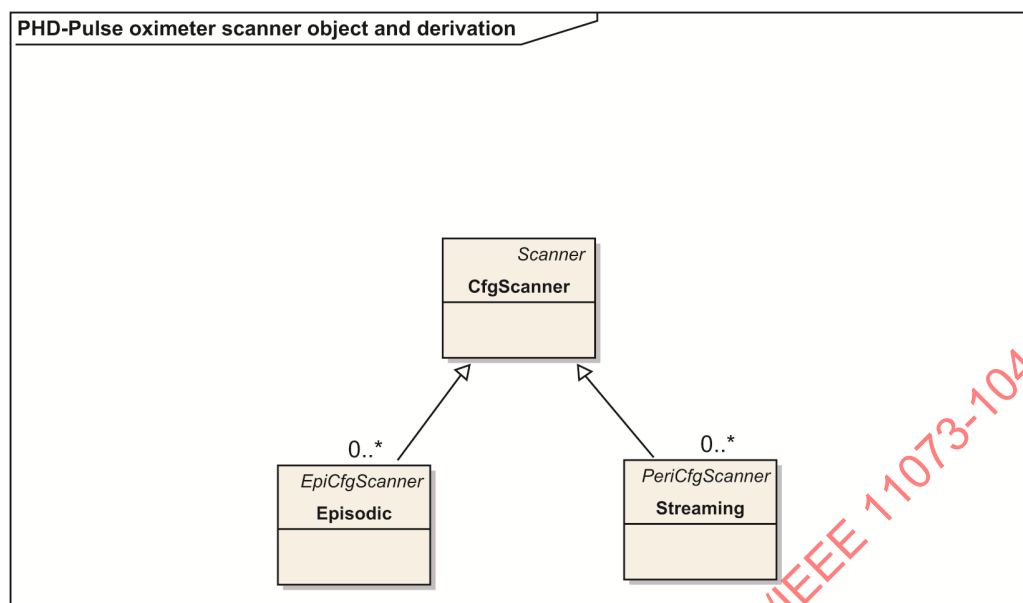


Figure 4—Pulse oximeter DIM for the periodic configurable scanner object

6.10.2 Periodic configurable scanner attributes

Table 18 shows the attributes applicable to the periodic configurable scanner object.

Table 18—Periodic configurable scanner object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Operational-State	See IEEE Std 11073-20601-2019.	M
Scan-Handle-List	See IEEE Std 11073-20601-2019.	C
Scan-Handle-Attr-Val-Map	See IEEE Std 11073-20601-2019.	C
Confirm-Mode	See IEEE Std 11073-20601-2019.	M
Confirm-Timeout	See IEEE Std 11073-20601-2019.	C
Transmit-Window	See IEEE Std 11073-20601-2019.	O
Reporting-Interval	See IEEE Std 11073-20601-2019.	M
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

With regard to the Confirm-Mode attribute, an agent may support either or both confirmed or unconfirmed scan reports; the manager shall support both confirmed and unconfirmed scan reports.

One or more periodic configurable scanner objects may be employed by a pulse oximeter in order to greatly increase the efficiency of delivering physiological and device information to the manager.

The events in Table 19 define the events sent by the pulse oximeter's periodic configurable scanner object.

Table 19—Periodic configurable scanner object events

Event	Mode	Event type	Event info parameter	Event-reply-info
Buf-Scan-Report-Var	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_VAR	ScanReportInfoVar	—
Buf-Scan-Report-Fixed	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_FIXED	ScanReportInfoFixed	—
Buf-Scan-Report-Grouped	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_GROUPED	ScanReportInfoGrouped	—
Buf-Scan-Report-MP-Var	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar	—
Buf-Scan-Report-MP-Fixed	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—
Buf-Scan-Report-MP-Grouped	Confirmed or unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_MP_GROUPED	ScanReportInfoMPGrouped	—

6.10.3 Episodic configurable scanner attributes

Table 20 shows the attributes applicable to the episodic configurable scanner object.

Table 20—Episodic configurable scanner object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601-2019.	M
Operational-State	See IEEE Std 11073-20601-2019.	M
Scan-Handle_list	See IEEE Std 11073-20601-2019.	C
Scan-Handle-Attr-Val-Map	See IEEE Std 11073-20601-2019.	C
Confirm-Mode	See IEEE Std 11073-20601-2019.	M
Confirm-Timeout	See IEEE Std 11073-20601-2019.	C
Transmit-Window	See IEEE Std 11073-20601-2019.	O
Min-Reporting-Interval	See IEEE Std 11073-20601-2019.	M
NOTE 1—See IEEE Std 11073-20601-2019 for information on whether an attribute is static or dynamic.		
NOTE 2—See 6.3 for a description of the qualifiers.		

With regard to the Confirm-Mode attribute, an agent may support either or both confirmed or unconfirmed scan reports. The manager shall support both confirmed and unconfirmed scan reports.

One or more episodic configurable scanner objects may be employed by a pulse oximeter in order to greatly increase the efficiency of delivering physiological and device information to the manager.

The events in Table 21 define the events sent by the pulse oximeter's episodic configurable scanner object.

Table 21—Episodic configurable scanner object events

Event	Mode	Event type	Event info parameter	Event-reply-info
Unbuf-Scan-Report-Var	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_VAR	ScanReportInfoVar	—
Unbuf-Scan-Report-Fixed	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_FIXED	ScanReportInfoFixed	—
Unbuf-Scan-Report-Grouped	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_GROUPED	ScanReportInfoGrouped	—
Unbuf-Scan-Report-MP-Var	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar	—
Unbuf-Scan-Report-MP-Fixed	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—
Unbuf-Scan-Report-MP-Grouped	Confirmed or unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_GROUPED	ScanReportInfoMPGrouped	—

6.11 Class extension objects

In this standard, no class extension objects are defined with respect to IEEE Std 11073-20601-2019.

6.12 Pulse oximeter information model extensibility rules

The pulse oximeter DIM of this standard may be extended by including vendor-specific metrics and attributes as required. Any object or attribute extensions implemented should follow the guidelines of this standard as closely as possible. Such vendor-specific attributes shall be identified by assigning nomenclature codes from the private numbering space (0xF000 – 0xFFFF) within the corresponding partition as defined in IEEE Std 11073-20601-2019.

A pulse oximeter agent having a configuration with extensions beyond the standard configuration, as specified in this standard, shall use a configuration ID in the range of IDs reserved for extended configurations (see IEEE Std 11073-20601-2019).

7. Pulse oximeter service model

7.1 General

The service model defines the conceptual mechanisms for data exchange services. These services are mapped to messages that are exchanged between the agent and manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. See IEEE Std 11073-20601-2019 for a detailed description of the PHD service model. The following subclauses define the specifics of object access and event reporting services for a pulse oximeter agent according to this standard.

7.2 Object access services

The object access services of IEEE Std 11073-20601-2019 are used to access the objects defined in the DIM of the pulse oximeter.

The following generic object access services are supported by a pulse oximeter agent according to this standard:

- GET service: used by the manager to retrieve the values of the agent MDS object and PM-store object attributes. The list of pulse oximeter MDS object attributes is given in 6.5.4.1.
- SET service: used by the manager to set the values of the agent object attributes. If the agent supports scanner objects, then the SET service shall be supported. If the agent does not support scanner objects, the SET service is optional. Note that although MDS attributes may be set, this standard does not allow the use of settable attributes as a mechanism for remote control.
- EVENT REPORT service: used by the agent to send configuration reports and measurement data to the manager. The list of event reports for the pulse oximeter device specialization is given in Table 3, Table 16, and Table 19.
- ACTION service: used by the manager to invoke actions (or methods) supported by the agent. An example is Set-Time action which is used to set a real-time clock with the absolute time at the agent.

Table 22 summarizes the object access services described in this standard.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10404:2022

Table 22 —Pulse oximeter object access services

Service	Subservice type name	Mode	Subservice type	Parameters	Result	Remarks
GET	<na>	<implied Confirmed>	<na>	GetArgumentSimple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list	Allows the manager to retrieve the value of an attribute of an object in the agent.
	<na>	<implied Confirmed>	<na>	GetArgumentSimple = (obj-handle = handle of PM-store object), attribute-id-list <optional>	GetResultSimple = (obj-handle = handle of PM-store object), attribute-list	Allows the manager to retrieve the values of all PM- store object attributes.
EVENT REPORT	MDS-Configuration- Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp	Configuration report to inform manager of the configuration of the agent.
	MDS-Scan-Report- Var	Confirmed or Unconfirmed	MDC_NOTI_SCAN_ REPORT_VAR	ScanReportInfoVar		Data report to provide dynamic data to manager for some or all of the agent's objects in variable format.
	MDS-Scan-Report- Fixed	Confirmed or Unconfirmed	MDC_NOTI_SCAN_ REPORT_FIXED	ScanReportInfoFixed		Data report to provide dynamic data to manager for some or all of the agent's objects in fixed format.
	MDS-Scan-Report MP-Var	Confirmed or Unconfirmed	MDC_NOTI_SCAN_ REPORT_MP_VAR	ScanReportInfoMPVar		This is the same as MDS- Dynamic-Data-Update-Var, but allows inclusion of data from multiple people.
	MDS-Scan-Report- MP-Fixed	Confirmed or Unconfirmed	MDC_NOTI_SCAN_ REPORT_MP_FIXED	ScanReportInfoMPFixed		
	Segment-Data-Event	Confirmed	MDC_NOTI_SEGMENT_ DATA	SegmentDataEvent	SegmentDataResult	
	Buf-Scan-Report-Var	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_ REPORT_VAR	ScanReportInfoVar		
	Buf-Scan-Report- Fixed	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_ REPORT_FIXED	ScanReportInfoFixed	—	
	Buf-Scan-Report- Grouped	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_ REPORT_GROUPED	ScanReportInfoGrouped	—	
	Buf-Scan-Report-MP- Var	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_ REPORT_MP_VAR	ScanReportInfoMPVar		
	Buf-Scan-Report-MP- Fixed	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_ REPORT_MP_FIXED	ScanReportInfoMPFixed	—	

Table 22—Pulse oximeter object access services (continued)

Service	Subservice type name	Mode	Subservice type	Parameters	Result	Remarks
ACTION	Buf-Scan-Report-MP-Grouped	Confirmed or Unconfirmed	MDC_NOTI_BUF_SCAN_REPORT_MP_GROUPED	ScanReportInfoMPGrouped	—	
	Unbuf-Scan-Report-Var	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_VAR	ScanReportInfoVar		
	Unbuf-Scan-Report-Fixed	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_FIXED	ScanReportInfoFixed	—	
	Unbuf-Scan-Report-Grouped	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_GROUPED	ScanReportInfoGrouped	—	
	Unbuf-Scan-Report-MP-Var	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar		
	Unbuf-Scan-Report-MP-Fixed	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—	
	Unbuf-Scan-Report-MP-Grouped	Confirmed or Unconfirmed	MDC_NOTI_UNBUF_SCAN_REPORT_MP_GROUPED	ScanReportInfoMPGrouped	—	
	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke		Manager method to invoke the agent to set time to requested value.
	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTimeInvoke	—	Manager method to invoke the agent to set time to requested value.
	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	—	
SET	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList	
	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmDataXferReq	TrigSegmDataXferRs	Allows the manager to begin sending segment data.
	<na>		<na>	SetArgumentSimple		Allows the manager to control the operational state of a scanner object.

7.3 Object access EVENT REPORT services

The EVENT REPORT service (see Table 22) is used by the agent to report its information (e.g., measurements). Event reports in this standard are a property of the MDS object only. The event reports used in this standard are defined in IEEE Std 11073-20601-2019.

The following conditions apply for a pulse oximeter agent according to this standard:

- Event reports transmitting measurement data may be used either in confirmed or unconfirmed mode.
- Some agent implementations support agent-initiated mode only through MDS object emission. These implementations should take care to not send any relatively high-bandwidth measurements such as plethysmogram data in this manner.
- Some agent implementations support agent-initiated mode only through the use of periodic or episodic configurable scanner objects. The manager shall be aware of the behavior of scanner object data transfer by controlling the Operational-State attribute of the appropriate scanner object.

A pulse oximeter agent designed to operate in an environment where data may be collected from multiple people may use one of the multiple-person event report styles to transmit all the data from each person in a single event. If this functionality is not required, the agent may use the single-person event report styles, which have reduced overhead.

A manager shall support both single-person and multiple-person event reports. A pulse oximeter agent shall support single-person event reports and may support multiple-person event reports. The formats for single and multiple-person reports are described in IEEE Std 11073-20601-2019.

8. Pulse oximeter communication model

8.1 Overview

The following subclauses describe the general communication model and procedures of the pulse oximeter agent as defined in IEEE Std 11073-20601-2019. Therefore, the respective parts of IEEE Std 11073-20601-2019 are not reproduced, rather the specific choices and restrictions with respect to optional elements (e.g., attributes and procedures) and specific extensions (e.g., nomenclature terms) are specified.

For an illustrative overview of the various message transactions during a typical measurement session, see the sequence diagram for the example use case in Annex D and the corresponding protocol data unit (PDU) examples in Annex E.

8.2 Communications characteristics

For a pulse oximeter agent implementing no other device specialization except this standard, the maximum size of an application protocol data unit (APDU) sent using medical device encoding rules (MDER) shall be not larger than N_{tx} . For this standard, $N_{tx} = 9216$ octets, based on the maximum APDU size that could be expected from a pulse oximetry agent implementing persistent metric capability (see 6.9.5). In the absence of the persistent metric capability, $N_{tx} = 5120$ octets, based on the maximum APDU size that could be expected from a pulse oximetry agent allowing sufficient capacity for several OCTET STRING entities within the MDS Production Specification attribute. An agent according to this definition shall be capable of receiving an APDU using MDER up to the size of at least N_{rx} . For this standard, $N_{rx} = 240$ octets, based on an Association Response with an allowance for a set of information in the option-list element of the PHDAssociationInformation structure of an Association Request.

If an agent implementing this device specialization implements functions from other device specializations, the following upper bound estimates for transmitted and received APDUs may serve as guidance:

An agent shall not transmit any APDU larger than the sum of N_{tx} of all the device specializations implemented and shall be capable of receiving any APDU up to the sum of N_{rx} of all the device specializations implemented. If these numbers are higher than the maximum size determined in IEEE Std 11073-20601-2019, the latter shall be applied.

8.3 Association procedure

8.3.1 General

Unless otherwise stated, the association procedure for a pulse oximetry agent and manager according to this standard shall be pursued as specified in IEEE Std 11073-20601-2019.

Table 23 lists the valid combinations of protocol version and nomenclature version. In the association procedure, an agent indicating support to a specific protocol version shall indicate support to the corresponding nomenclature version as well. In the association procedure, a manager selecting a specific protocol version shall select the corresponding nomenclature version.

Table 23—Valid combinations of protocol and nomenclature version

Protocol version	Bit value	Corresponding nomenclature version	Bit value
1	0x80000000	1	0x80000000
2	0x40000000	1	0x80000000
3	0x20000000	2	0x40000000
4	0x10000000	3	0x20000000

To indicate support for multiple protocol versions, the bit values are combined. For example, if the agent supports protocol-version2, protocol-version3 and protocol-version4, it shall use protocol version bits 0x70000000 and nomenclature-version bits 0xE0000000.

Future versions of this specification may include further valid combinations that can be used by implementations that comply with that future version.

8.3.2 Agent procedure—Association request

In the Association Request message sent by the agent to the manager, the following points apply:

- The version of the association procedure used by the agent shall be set to *assoc-version1* (i.e., *assoc-version* = 0x80000000).
- The *DataProtoList* structure element of the data protocol identifier shall be set to *data-proto-id-20601* (i.e., *data-proto-id* = 0x5079).
- The *data-proto-info* field shall contain a Phd Association Information structure, which shall contain the following parameter values:
 - The version of the data exchange protocol shall be set to *protocol-version4* (i.e., *protocol-version* = 0x10000000). Support for any other version may be indicated by setting additional bits. When protocols lower than *protocol-version4* are used, the agent shall use only features in that protocol.
 - At least the MDER shall be supported (i.e., *encoding-rules* = 0x8000).
 - The protocol version bits and nomenclature version bits shall consist of valid combinations of bits as defined in Table 23.

- The *functional-units* field may have the test association bits set, but shall not have any other bits set.
- The *system-type* field shall be set to sys-type-agent (i.e., *system-type* = 0x00800000).
- The *system-id* field shall be set to the value of the System-Id attribute of the MDS object of the agent. The manager may use this field to determine the identity of the pulse oximeter with which it is associating and, optionally, to implement a simple access restriction policy.
- The *dev-config-id* field shall be set to the value of the Dev-Configuration-Id attribute of the MDS object of the agent.

If the agent supports only the pulse oximeter specialization, then the field indicating the data request modes (data-req-mode-capab) supported by the pulse oximeter agent shall be set based on the communication capabilities of the agent.

If the agent supports agent-initiated measurement transfer, then data-req-mode-capab shall have the data-req-supp-init-agent bit set. The data-req-init-manager-count shall be set to zero, and data-req-init-agent-count shall be set to 1.

8.3.3 Manager procedure—Association response

In the Association Response message sent by the manager, the following points apply:

- The result field shall be set to an appropriate response from the responses defined in IEEE Std 11073-20601-2019. For example, if all other conditions of the association protocol are satisfied, *accepted* is returned when the manager recognizes the *dev-config-id* of the agent and *accepted-unknown-config* otherwise.
- In the DataProtoList structure element, the data protocol identifier shall be set to data-proto-id-20601 (i.e., *data-proto-id* = 0x5079).
- The *data-proto-info* field shall be filled in with a Phd Association Information structure, which shall contain the following parameter values:
 - The manager following this specialization shall support protocol-version4. The manager may support additional protocol versions and select them if the agent offers them. When protocols lower than protocol-version4 are used, the manager shall use only features in that protocol.
 - The manager shall respond with a single selected encoding rule that is supported by both agent and manager. The manager shall support at least the MDER.
 - The manager shall select a valid combination of protocol version and nomenclature version as defined in Table 23.
- The *functional-units* field shall have all bits reset except for those relating to a test association.
- The *system-type* field shall be set to sys-type-manager (i.e., *system-type* = 0x80000000).
- The *system-id* field shall contain the unique system ID of the manager device, which shall be a valid EUI-64 type identifier.
- The *dev-config-id* field shall be manager-config-response (0).
- The data-req-mode-capab-flags field shall be 0.
- The *data-req-init-*-count* fields shall be 0.

8.4 Configuring procedure

8.4.1 General

The agent enters the Configuring state if it receives an Association Response of *accepted-unknown-config*. In this case, the configuration procedure as specified in IEEE Std 11073-20601-2019 shall be followed. The following subclauses specify the configuration notification and response messages for a pulse oximetry agent with standard configuration ID 0x0192. Normally, a manager would already know the standard configuration. However, for the purposes of this example, it does not.

8.4.2 Pulse oximeter—Standard configuration

8.4.2.1 Agent procedure

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an MDC_NOTI_CONFIG event to send its configuration to the manager (see IEEE Std 11073-20601-2019). The ConfigReport structure is used for the event-info field (see Table 3). For a pulse oximetry agent with standard configuration ID 0x0192, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x70	CHOICE.length = 112
0x00 0x6E	OCTET STRING.length = 110
0x12 0x35	invoke-id (differentiates this from other outstanding messages)
0x01 0x01	CHOICE(Remote Operation Invoke Confirmed Event Report)
0x00 0x68	CHOICE.length = 104
0x00 0x00	obj-handle = 0 (MDS object)
0xFF 0xFF 0xFF 0xFF	event-time = 0xFFFFFFFF
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x56	event-info.length = 86 (start of ConfigReport)
0x01 0x92	config-report-id = 0x0192
0x00 0x02	config-obj-list.count = 2 Measurement objects will be “announced”
0x00 0x58	config-obj-list.length = 88
0x00 0x06	obj-class = MDC_MOC_VMO_METRIC_NU
0x00 0x01	obj-handle = 1 (→ 1 st Measurement is SpO ₂)
0x00 0x04	attributes.count = 4
0x00 0x24	attributes.length = 36
0x09 0x2F	attribute-id = MDC_ATTR_ID_TYPE
0x00 0x04	attribute-value.length = 4
0x00 0x02 0x4B 0xB8	MDC_PART_SCADA MDC_PULS_OXIM_SAT_O2
0x0A 0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00 0x02	attribute-value.length = 2
0x40 0x40	avail-stored-data, acc-agent-init, measured
0x09 0x96	attribute-id = MDC_ATTR_UNIT_CODE
0x00 0x02	attribute-value.length = 2
0x02 0x20	MDC_DIM_PERCENT
0x0A 0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00 0x08	attribute-value.length = 8
0x00 0x01	AttrValMap.count = 1
0x00 0x04	AttrValMap.length = 4
0x0A 0x4C 0x00 0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x0A 0x82 0x00 0x08	MDC_ATTR_TIME_STAMP_BO value length = 8

0x00 0x06	obj-class = MDC_MOC_VMO_METRIC_NU
0x00 0x0A	obj-handle = 10 (→2 nd Measurement is pulse rate)
0x00 0x04	attributes.count = 4
0x00 0x24	attributes.length = 36
0x09 0x2F	attribute-id = MDC_ATTR_ID_TYPE
0x00 0x04	attribute-value.length = 4
0x00 0x02 0x48 0x1A	MDC_PART_SCADA MDC_PULS_OXIM_PULS_RATE
0x0A 0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00 0x02	attribute-value.length = 2
0x40 0x40	avail-stored-data, acc-agent-init, measured
0x09 0x96	attribute-id = MDC_ATTR_UNIT_CODE
0x00 0x02	attribute-value.length = 2
0x0A 0xA0	MDC_DIM_BEAT_PER_MIN
0x0A 0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00 0x08	attribute-value.length = 8
0x00 0x01	AttrValMap.count = 1
0x00 0x04	AttrValMap.length = 4
0x0A 0x4C 0x00 0x02	MDC_ATTR_NU_VAL_OBS_BASIC, 2
0x0A 0x82 0x00 0x08	MDC_ATTR_TIME_STAMP_BO value.length = 8

8.4.2.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response Confirmed Event Report” data message with an MDC_NOTI_CONFIG event using the ConfigReportRsp structure for the event-info field (see Table 3). An example configuration notification response message (corresponding to the configuration notification request message described in 8.4.2.1) can be seen as follows:

0xE7 0x00	APDU CHOICE Type (PrstAdu)
0x00 0x16	CHOICE.length = 22
0x00 0x14	OCTET STRING.length = 20
0x12 0x35	invoke-id = 0x1235 (mirrored from invocation)
0x02 0x01	CHOICE (Remote Operation Response Confirmed Event Report)
0x00 0x0E	CHOICE.length = 14
0x00 0x00	obj-handle = 0 (MDS object)
0x00 0x00 0x00 0x00	currentTime = 0
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x04	event-reply-info.length = 4
0x01 0x92	ConfigReportRsp.config-report-id = 0x0192
0x00 0x00	ConfigReportRsp.config-result = accepted-config

8.5 Operating procedure

8.5.1 General

Measurement data and status information are communicated from the pulse oximetry agent during the Operating state. If not stated otherwise, the operating procedure for a pulse oximetry agent of this standard shall be as specified in IEEE Std 11073-20601-2019.

8.5.2 GET pulse oximeter MDS attributes

See Table 4 for a summary of the GET service.

If the manager leaves the attribute-id-list field in the roiv-cmip-get service message empty, the pulse oximetry agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of all implemented attributes of the MDS object.

If the manager requests specific MDS object attributes, indicated by the elements in attribute-id-list, the pulse oximetry agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of the requested attributes of the MDS object that are implemented.

8.5.3 Measurement data transmission

See Table 3, Table 16, and Table 19 for a summary of the EVENT REPORT services available for measurement data transfer.

Measurement data transfer for a pulse oximetry agent of this standard is initiated by the agent; however the manager may control transmission of data through use of the scanner object. To limit the amount of data being transported within an APDU, the pulse oximetry agent shall not include more than 25 temporarily stored measurements in a single event report. If more than 25 pending measurements are available for transmission, they may be sent either using multiple event reports or by incorporating a persistent store facility. If multiple oximetry measurements are available, up to 25 measurements should be transmitted within a single event report. Alternatively, they may be transmitted using a single event report for each oximetry measurement. However, the former strategy is recommended to reduce overall message size and power consumption.

8.6 Time synchronization

Time synchronization may be employed between a pulse oximetry agent and a manager to coordinate the clocks used when reporting physiological events. Note that the mechanism for synchronizing an agent to a manager is outside the scope of this standard. If time synchronization is used, then this shall be reported in the Mds-Time-Info attribute of the MDS object.

9. Test associations

A pulse oximeter may implement a wide range of behaviors in a test association that enable a manufacturer to test features of a product in a comprehensive manner. It is also possible for a pulse oximeter to not support test associations at all. This clause defines a simple behavior that simulates the generation of a measurement in the context of a standard device configuration.

9.1 Behavior with standard configuration

In order to facilitate automated standardized test processes, a pulse oximeter that presents the standard configuration ID and enters into a test association should be able to simulate the arrival of measurement data from the device sensors. It should not be necessary for an operator to stimulate the sensors in order for the measurement data to be generated.

After the agent enters the Operating state, it simulates the reception of an event from the sensors representing an SpO₂ measurement of 123% and a pulse rate of 456 beats per minute. To the extent possible, this measurement is seen only by those components of the agent that understand the test association. When the event is propagated into a numeric object, the test-data bit of the measurement-status attribute shall be set if the measurement-status attribute is supported. An agent is not required to use the measurement-status attribute if it would not normally do so outside of a test association.

The agent should send the events reports for all simulated measures within 30 s of entering the Operating state. The test association is terminated in a manner consistent with the agent's normal behavior for terminating an association.

9.2 Behavior with extended configurations

This specification does not define a test association that uses an extended configuration.

10. Conformance

10.1 Applicability

This standard shall be used in conjunction with IEEE Std 11073-20601-2019.

An implementation or a system can conform to the following elements of this standard:

- DIM class hierarchy and object definitions (object attributes, notifications, methods, and data type definitions)
- Nomenclature code values
- Protocol and service models
- Communication service model (association and configuration)

10.2 Conformance specification

This standard offers levels of conformance with respect to strict adherence to the standard device and the use of extensions for the following:

- Information model of a specific device
- Use of attributes, value ranges, and access methods

A vendor shall specify the level of conformance for an implementation based on this standard and provide details of the way in which the definitions of this standard and any extensions are applied.

Specifications shall be provided in the form of a set of ICSs as detailed in 10.4.

Since this standard is used in conjunction with IEEE Std 11073-20601-2019, the ICS should be created for this standard first. The ICS created for IEEE Std 11073-20601-2019 may then refer to the ICS for this standard where applicable.

10.3 Levels of conformance

10.3.1 General

This standard defines two levels of conformance in 10.3.2 and 10.3.3.

10.3.2 Conformance Level 1: Base conformance

The application uses elements of the information, service, and communication models (object hierarchy, actions, event reports, and data type definitions) and the nomenclature scheme defined in IEEE Std 11073-20601-2019 and the ISO/IEEE P11073-104zz standards. All mandatory features defined in the object definition tables and in the ICS tables are implemented. Further, any conditional, recommended, or optional features that are implemented shall follow the requirements in IEEE Std 11073-20601-2019 and the ISO/IEEE P11073-104zz standards.

10.3.3 Conformance Level 2: Extended nomenclature (ASN.1 and/or IEEE 11073-10101)

Conformance Level 2 meets conformance level 1, but also uses or adds extensions in at least one of the information, service, communication, or nomenclature models. These extensions shall conform to nomenclature codes from ASN.1 and/or within the IEEE 11073-10101 framework (0xF000 – 0xFFFF). These extensions should be defined in ICS tables pointing towards their reference.

10.4 Implementation conformance statements (ICSs)**10.4.1 General format**

The ICSs are provided as an overall conformance statement document that comprises a set of specific ICS tables in the form given by the templates in 10.4.2 through 10.4.6.

Each ICS table has the following columns:

Index	Feature	Reference	Req./Status	Support	Comment
-------	---------	-----------	-------------	---------	---------

The table column headings have the following meanings:

- Index, which is an ID (e.g., a tag) of a specific feature.
- Feature, which briefly describes the characteristic for which a conformance statement is being made.
- Reference, which is to the clause or subclause within this standard or an external source for the definition of the feature (may be empty).
- Req./Status, which specifies the conformance requirement (e.g., mandatory or recommended). In some cases, this standard does not specify conformance requirements, but requests that the status of a particular feature be provided.
- Support, which specifies the presence or absence of a feature and any description of the characteristics of the feature in the implementation. This column is to be filled out by the implementer.
- Comment, which contains any additional information on the feature. This column is to be filled out by the implementer.

10.4.2 General ICS

The general ICS specifies the versions/revisions that are supported by the implementation and high-level system behavior.

Table 24 shows the general ICS.

Table 24—IEEE 11073-10404 general ICS

Index	Feature	Reference	Req./Status	Support	Comment
GEN 11073-10404-1	Implementation Description	—	Identification of the device/application. Description of functionality.		
GEN 11073-10404-2	Standards Followed and Their Revisions	(standard documents)	(set of existing revisions)	(set of supported revision)	
GEN 11073-10404-3	Nomenclature Document Used and Revision	(standard documents)	(set of existing revisions)	(set of supported revisions)	
GEN 11073-10404-4	Conformance Adherence - Level 1 -	See 10.3.2	Base conformance declaration that device meets the following IEEE 11073-10404 conformance requirements: A) All mandatory requirements shall be implemented. B) If implemented, conditional, recommended, and optional requirements shall conform to this standard.	Yes/No (No is not expected as no implies that the implementation is NON-conformant)	
GEN 11073-10404-5	Conformance Adherence - Level 2 -	See 10.3.3	In addition to GEN 11073-10404-4, if the device implements extensions and/or additions, they shall conform to nomenclature codes from ASN.1 and/or IEEE 11073-10101 framework. These extensions should also be defined in ICS tables pointing towards their reference.	Yes/No	
GEN 11073-10404-6	Object Containment Tree	See 6.3	Provide object containment diagram showing relations between object instances used by the application. A conforming implementation uses only object relations as defined in the DIM.		
GEN 11073-10404-7	Nomenclature Document Used and Revision	(standard documents)	(set of existing revisions)	(set of supported revision)	
GEN 11073-10404-8	Data Structure Encoding	—	—	description of encoding method(s) for ASN.1 data structures	
GEN 11073-10404-9	Use of Private Objects	—	Does the implementation use objects that are not defined in the DIM?	Yes/No [If yes: explain in Table 25]	
GEN 11073-10404-10	Use of Private Nomenclature Extensions	—	Does the implementation use private extensions to the nomenclature (i.e., 0xF000–0xFFFF codes from IEEE 11073-10101)? Private nomenclature extensions are allowed <i>only</i> if the standard nomenclature does not include the specific terms required by the application.	Yes/No [If yes: explain in the Table 28]	
GEN 11073-10404-11	IEEE Std 11073-20601 Conformance		Provide the conformance report required by IEEE Std 11073-20601-2019.		

10.4.3 DIM MOC ICS

The DIM MOC ICS defines which objects are implemented. Information on each object shall be provided as a separate row in the template of Table 25.

Table 25—Template for DIM MOC ICS

Index	Feature	Reference	Req./Status	Support	Comment
MOC- <i>n</i>	Object description	Reference to the clause in this standard or other location where the object is defined.	Implemented	Specify restrictions, e.g., maximum number of supported instances.	

The *n* in the Index column should be the object handle for implementations that have predefined objects. Otherwise, the Index column shall be simply a unique number (1..*m*).

All private objects should be specified and include a reference to the definition for the object. Where no publicly available reference is available, the definition of the object should be appended to the conformance statement.

The Support column should indicate any restrictions for the object implementation.

An object containment diagram (class instance diagram) should be provided as part of the DIM MOC ICS.

10.4.4 MOC attribute ICS

For each supported object as defined in the DIM MOC ICS, a MOC attribute ICS has to be provided that defines which attributes are used/supported by the implementation, including any inherited attributes. Table 26 is a template only.

Table 26—Template for MOC attribute ICS

Index	Feature	Reference	Req./Status	Support	Comment
ATTR- <i>n-x</i>	Attribute Name. Extended attributes shall include the Attribute ID also.	Fill in the reference to the ASN.1 structure if the attribute is not defined in this standard.	M = Mandatory/ C = Conditional/ R = Recommended/ O = Optional [as per definition in attribute definition tables]	Implemented? Yes/No Static/Dynamic Specify restrictions, e.g., value ranges. Describe how attribute is accessed (e.g., Get, Set, sent in config event report, sent in a data event report) Describe any specific restrictions.	

All private attributes should be specified and include reference to the definition for the attribute. Where no publicly available reference is available, the definition of the attribute should be appended to the conformance statement.

The Support column shall specify whether the attribute is implemented; for extension attributes, whether the attribute value is static or dynamic; any value ranges; restrictions on attribute access or availability; and any other information.

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the MOC ICS). There is one separate table for each supported managed object.

The *x* in the Index column is a unique serial number (1..*m*).

10.4.5 MOC notification ICS

The MOC notification ICS specifies all implemented notifications (typically in form of the EVENT REPORT service) that are emitted by the agent. Table 27 provides a template for use. One table has to be provided for each object that supports special object notifications.

Table 27—Template for MOC notification ICS

Index	Feature	Reference	Req./Status	Support	Comment
NOTI- <i>n</i> - <i>x</i>	Notification Name and Notification ID	Reference to the clause in this standard or other location where the event is defined.		The Support column shall specify how the notification is sent and any restrictions.	

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the MOC ICS). There is one separate table for each managed object that supports specific object notifications (i.e., events).

The *x* in the Index column is a unique serial number (1..*m*).

All private notifications should be specified and include reference to the definition for the notification. Where no publicly available reference is available, the definition of the notification should be appended to the conformance statement.

10.4.6 MOC nomenclature ICS

The MOC nomenclature ICS specifies all nonstandard nomenclature codes that are utilized by the agent. Table 28 provides a template for use. One row of the table is to be used for each nomenclature element.

Table 28—Template for MOC nomenclature ICS

Index	Feature	Reference	Req./Status	Support	Comment
NOME- <i>n</i>	Nomenclature Name and Nomenclature value	Reference to the clause in this standard or other location where the nomenclature is defined or used.		Describe how the nomenclature is used. Describe any specific restrictions,	

The *n* in the Index column is a unique serial number (1..*m*).

Annex A

(informative)

Bibliography

[B1] Draft Guidance for Industry and FDA Staff – Pulse Oximeters – Premarket Notification Submissions [510(k)s], July 19, 2007.

[B2] IEC 60601-1, Ed. 3, Medical electrical equipment—Part 1: General requirements for basic safety and essential performance.⁸

[B3] IEC 60601-2 (all parts), Medical electrical equipment—Part 2: Particular requirements for the basic safety and essential performance for specific device.

[B4] IEC 62304 /EN 62304, Medical device software—Software life-cycle processes.

[B5] IEC 80001-1, Application of risk management for IT-networks incorporating medical devices—Part 1: Roles, responsibilities, and activities.

[B6] ISO/IEEE 11073-10201:2004, Health informatics—Point-of-care medical device communication—Part 10201: Domain information model.⁹

[B7] ISO/IEEE 11073-20101:2004, Health informatics—Point-of-care medical device communication—Part 20101: Application Profiles—Base Standard.

[B8] ISO 14971:2007, Medical devices—Application of risk management to medical devices.

[B9] ISO 80601-2-61:2017, Medical electrical equipment – Particular requirements for basic safety and essential performance of pulse oximeter equipment.

[B10] ITU-T Rec. X.680, Information technology – Abstract Syntax Notation One (ASN.1): Specification of basic notation.¹⁰

⁸ EN publications are available from the European Committee for Standardization (CEN) (<http://www.cenorm.be>).

⁹ ISO publications are available from the International Organization for Standardization (<https://www.iso.org/>) and the American National Standards Institute (<https://www.ansi.org/>).

¹⁰ ITU-T publications are available from the International Telecommunications Union (<http://www.itu.int/>).

Annex B

(normative)

Additional ASN.1 definitions

B.1 Device and sensor status bit mapping

The threshold extensions to the numeric class require the following four ASN.1 structure definition:

```
PulseOxDevStat ::= BITS-16 {  
    sensor-disconnected(0),  
    sensor-malfunction(1),  
    sensor-displaced(2),  
    sensor-unsupported(3),  
    sensor-off(4),  
    sensor-interference(5),  
    signal-searching(6),  
    signal-pulse-questionable(7),  
    signal-non-pulsatile(8),  
    signal-erratic(9),  
    signal-low-perfusion(10),  
    signal-poor(11),  
    signal-inadequate(12),  
    signal-processing-irregularity(13),  
    device-equipment-malfunction(14),  
    device-extended-update(15)  
}
```